
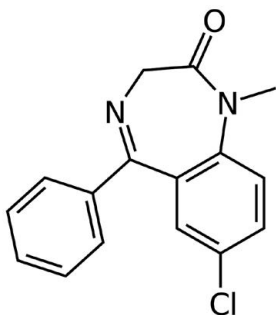


## Diazepam Tablet Analyzed with HPLC – AppNote

### Excellent Peak Shape and Precision for a Benzodiazepine Compound Valium®

This Isocratic Method shows how using 0.1% Trifluoroacetic Acid (*TFA*) in the Mobile Phase can produce a Peak with excellent Efficiency and Symmetry. In the USP Assay Method, System Suitability requires that a tailing factor of not more than 2.0 be obtained for the API, and this Method produces a Peak that is well within the Specification.

An overlay of Five consecutive chromatograms is shown in the Figure to illustrate the Precision and Robustness of the Method.

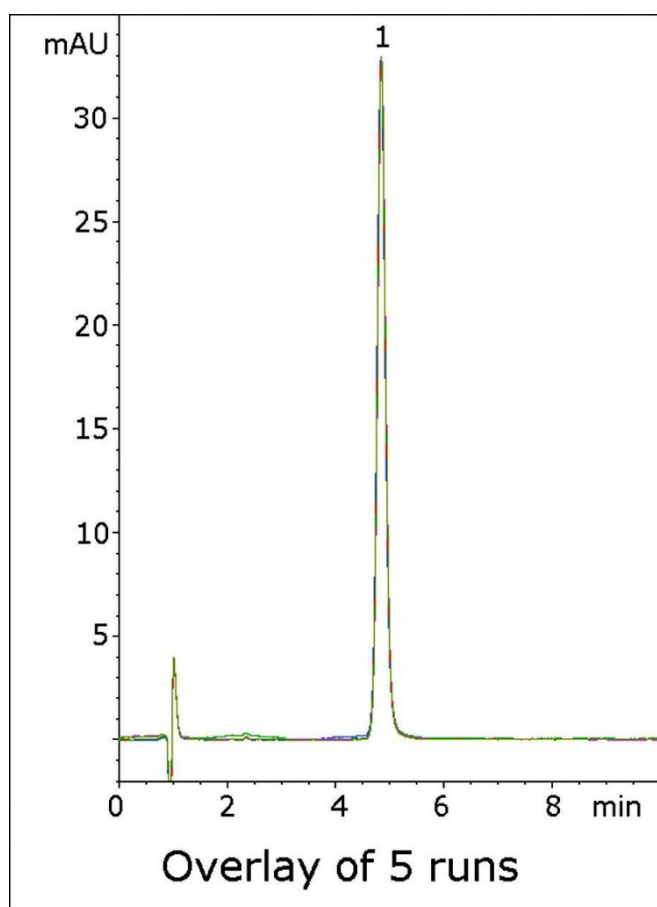

**Peak:**

Diazepam

## Method Conditions

**Column:** Cogent Bidentate C8™, 4µm, 100Å

**Catalog No.:** 40008-75P

**Dimensions:** 4.6 x 75mm

**Mobile Phase:** 70:30 DI Water / Acetonitrile with 0.1% Trifluoroacetic Acid (TFA) v/v

**Injection vol.:** 10µL

**Flow rate:** 1.0mL / minute

**Detection:** UV @ 254nm

**Sample Preparation:** 10mg of a ground Valium® tablet was added to a 10mL volumetric flask containing a portion of a 50:50 Acetonitrile / DI Water diluent. The flask was sonicated 10 minutes and diluted to mark. A portion was filtered with a 0.45µm Nylon Syringe Filter (MicroSolv Tech Corp.).

**to:** 0.9 minutes

**Note:** *Diazepam is a benzodiazepine used to treat conditions such as anxiety, muscle spasms, insomnia, seizures, and to control agitation caused by alcohol withdrawal. It is marketed as Valium® by Hoffmann-La Roche, although generic versions are currently available.*



## Attachment

**No 190 Diazepam Tablet Analyzed with HPLC pdf 0.3 Mb**

**MicroSolv Technology Corporation**

9158 Industrial Blvd. NE, Leland, NC 28451

tel. (732) 380-8900, fax (910) 769-9435

Email: [customers@mtc-usa.com](mailto:customers@mtc-usa.com)

Website: [www.mtc-usa.com](http://www.mtc-usa.com)