
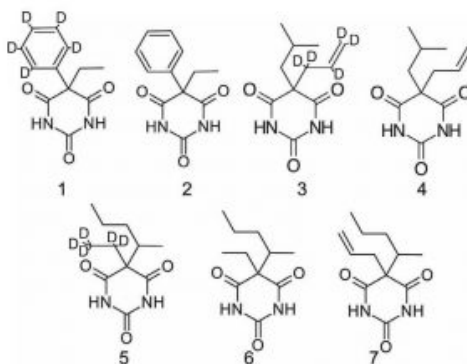


Barbiturates Analyzed with LCMS – AppNote

Standard Solutions in Human Urine Spiked with Barbiturates

After minimal sample preparation (*dilute-and-shoot approach*), spiked urine samples were analyzed using a C18 Column. The analysis was based on a Separation of Standards [1]. The obtained Peaks were Symmetrical ($As < 1.05$) and Efficient (> 106 pl/m). No shift in retention Times was observed after the samples were diluted ten-fold (*data not shown*). Matrix effects that would diminish the signal intensity were less than 5%.

This Method shows a possible Application for Analysis of these Compounds in Forensic Samples.

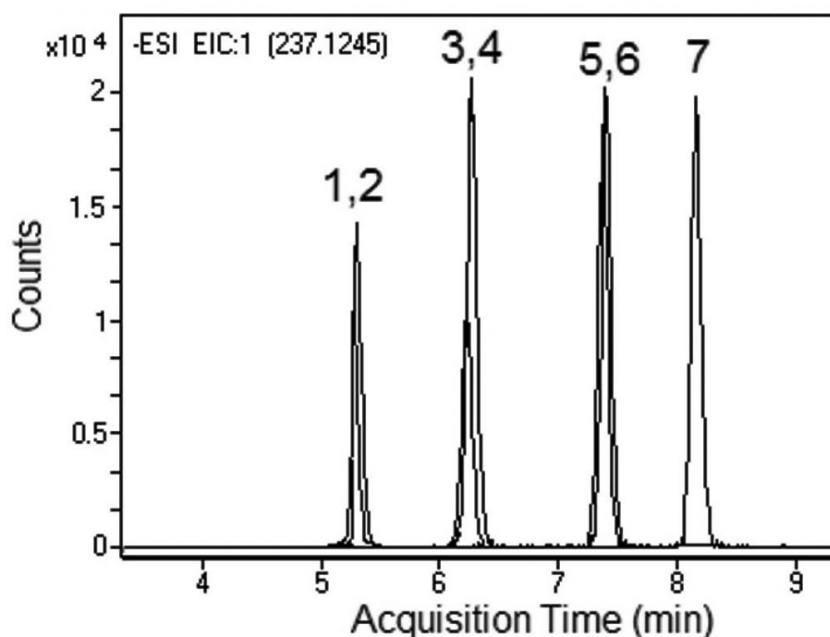

Peaks:

1. Phenobarbital-D5 $m/z = 236.1089$,
2. Phenobarbital $m/z = 231.0775$,
3. Butalbital-D5 $m/z = 228.1402$,
4. Butalbital $m/z = 223.1088$,
5. Pentobarbital-D5 $m/z = 230.1558$,
6. Pentobarbital $m/z = 225.1245$,
7. Secobarbital $m/z = 237.1245$

Method Conditions

Column: Cogent Bidentate C18™, 4µm, 100Å

Catalog No.: [40018-05P-2](#)

Dimensions: 2.1 x 50mm

Mobile Phase:

A: DI Water with 10mM Ammonium Formate

B: 95:5 Acetonitrile / DI Water with 10mM Ammonium Formate (v/v)

Gradient:

Time (minutes)	%B
0	10
1	10
10	45

Post Time: 3 minutes

Injection vol.: 1µL

Flow rate: 0.4mL / minute

Detection: ESI - NEG - Agilent 6210 MSD TOF Mass Spectrometer

Sample Preparation: Stock solutions of Barbiturates were prepared at a concentration of 1mg / mL in Methanol. Then 2mL of a urine sample was spiked with the stock solutions diluted, (*dilution 1:100*) and filtered through a 0.45µm Nylon Syringe Filter (MicroSolv Tech Corp.) into Autosampler Vials.

t₀: 0.3 minutes



[1] J.J. Pesek, M.T. Matyska, A.M. Kim, J. Sep. Sci. 2013, 36, 2760-2766.

Attachment

No 270 Barbiturates Analyzed with LCMS pdf 0.3 Mb [Download File](#)

MicroSolv Technology Corporation

9158 Industrial Blvd. NE, Leland, NC 28451

tel. (732) 380-8900, fax (910) 769-9435

Email: customers@mtc-usa.com

Website: www.mtc-usa.com