

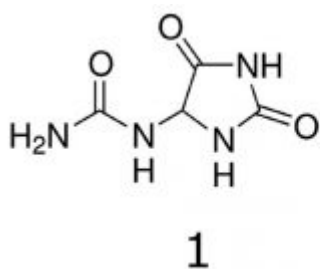


Uric Acid (UA) Metabolites Analyzed by LCMS – AppNote

Allantoin and 6-Aminouracil

The presented method for analysis of UA metabolites in human Urine is very simple and does not require Mobile Phase additives or pre-Column derivatization. The peaks are symmetrical and the MS signal is not diminished as is the case when Ammonium Formate or Acetate is used as the Mobile Phase additive.

The analyzed metabolites are signature end products for UA degradation in the presence of oxidants and can be used as biomarkers for different disease states.

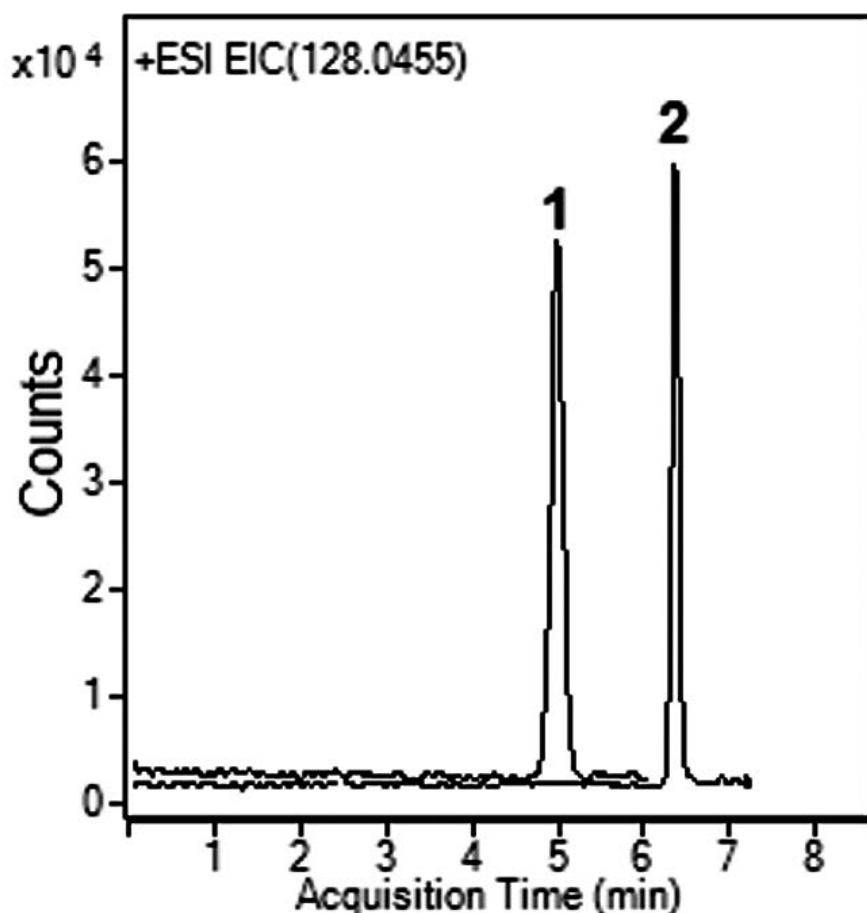

Peaks:

1. Allantoin 159.0513 m/z [M+H]⁺

2. 6-Aminouracil 128.0455 m/z [M+H]⁺

Method Conditions

Column: Cogent Diol™, 4μm, 100Å

Catalog No.: 40060-15P-3

Dimensions: 3.0 x 150mm

Mobile Phase:

A: DI Water / 0.1% Formic Acid (v/v)

B: Acetonitrile / 0.1% Formic Acid (v/v)

Gradient:

Time (minutes)	%B
0	95
1	95
6-7	30
8	95

Flow rate: 0.4 mL/minute

Detection: ESI - POS - Agilent 6210 MSD TOF Mass Spectrometer

Injection vol.: 1μL

Sample Preparation: 200 μL of Urine sample was centrifuged at 14,000 rpm for 10 minutes two times. The supernatant was diluted 1: 2 with Acetonitrile and centrifuged again at 14,000 rpm for 5 minutes. The filtrate was injected into LC-MS.

t₀: 0.9 minutes

Note: Humans lack the enzyme (Uricase) which converts UA to Allantoin. However the compound still can be detected in human Urine samples. UA can react with an oxidant in a step reaction and the end product is Allantoin. When UA is degraded, it can't be renewed. The presence of Allantoin in Urine is an indicator of a disease state (oxidative stress, renal failure, diabetes, etc.). The Allantoin/UA ratio is also elevated in Down syndrome and chronic lung disease. 6-Aminouracil is a direct product of reaction of UA with nitric oxide, which has a role in cardiovascular disease.



Attachment

No 290 Uric Acid Metabolites pdf 0.2 Mb [Download File](#)

Printed from the Chrom Resource Center
MicroSolv Technology Corporation
9158 Industrial Blvd. NE, Leland, NC 28451
tel. (732) 380-8900, fax (910) 769-9435
Email: customers@mtc-usa.com
Website: www.mtc-usa.com
Date: 04-05-2024