
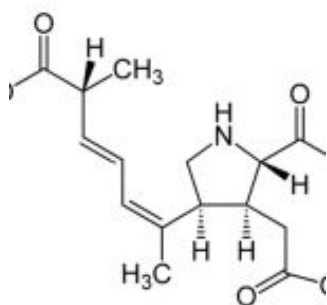


Domoic Acid separation with LCMS without derivatization – AppNote

Several analytical methods have been developed for the quantitative determination of Domoic Acid (DA). However, many of the methods require tedious and labor-intensive derivatization of this compound in order to detect it. A new method based on HPLC and MS detection which does not require derivatization has been developed. A simple linear gradient and typical MS compatible mobile phases were used to retain DA, a potent Neurotoxin.

The advantage of using Cogent Columns is that they equilibrate rapidly when a gradient is used. The method can be used by regulatory agencies responsible for monitoring the occurrence of toxins for analysis of Domoic Acid in seafood samples and other laboratories.

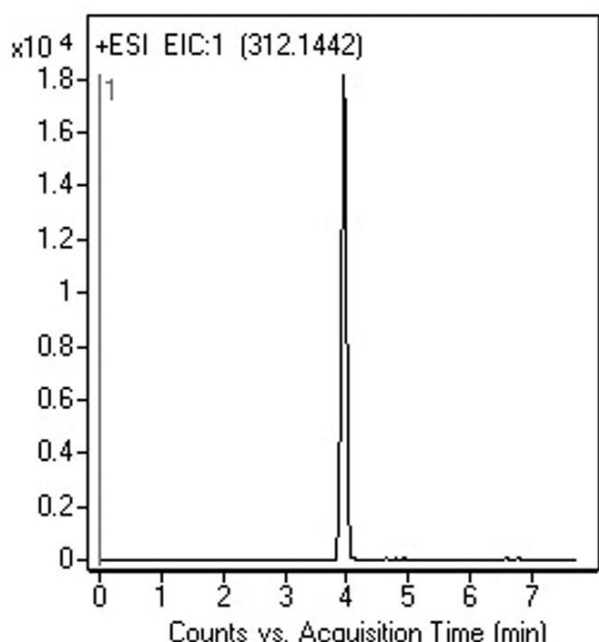

Peak:

Domoic Acid 312.1442 m/z (M + H)⁺

Method Conditions:

Column: Cogent Diamond Hydride™, 4μm, 100Å

Catalog No.: 70000-05P-2

Dimensions: 2.1 x 50 mm

Solvents:

A: 50% Methanol / 50% DI Water / 0.1% Formic Acid

B: 97% Acetonitrile / 3% DI Water / 0.1% Formic Acid

Gradient:

Time (Minutes)	%B
0	95
10	30
11	30
12	95

Post Time: 5 minutes

Injection Volume: 1 μ L

Flow Rate: 0.4 mL/minute

Detection: ESI – POS – Agilent 6210 MSD TOF Mass Spectrometer

Sample Preparation: The stock solution was prepared by dissolving 1.0 mg/mL DA in Methanol diluent. The stock was diluted using 50% solvent A and 50% solvent B mixture for the final concentration 0.5 mg/L. Before injection, solution was filtered using a 0.45 micron Nylon Filter (MicroSolv Tech Corp.).

Note: Domoic Acid, a compound known for over 50 years, was found to have neurological effects when ingested by humans. It is the chemical responsible for amnesiac shellfish poisoning (ASP). Upon ingestion by humans, it can cause diarrhea, dizziness, seizures, permanent loss of short-term memory, and even death. In Canada, the European Union, and the USA, the legal limit is 20 μ g DA/g in wet tissues of shellfish.

**Attachment**

Domoic Acid pdf [Download File](#)

Printed from the Chrom Resource Center

MicroSolv Technology Corporation

9158 Industrial Blvd. NE, Leland, NC 28451

tel. (732) 380-8900, fax (910) 769-9435

Email: customers@mtc-usa.com

Website: www.mtc-usa.com

Date: 05-07-2024