



## Sarcosine Analyzed with LCMS – AppNote


### Separation of Potential Urine Biomarker from Isobaric $\beta$ -Alanine

This developed LCMS method can separate Sarcosine from Beta- Alanine in serum and urine samples without using labor intensive sample derivatization. Since Sarcosine is considered a potential biomarker for prostate cancer risk and aggressiveness, it is essential to resolve and accurately quantify this compound in the presence of isobaric (same  $m/z$ ) Beta-Alanine.

The developed method is Sensitive, Specific, Quantitative, and Reproducible (%RSD = 0.1). It can be used in large scale studies with numerous samples (high throughput of the method due to simple sample preparation).

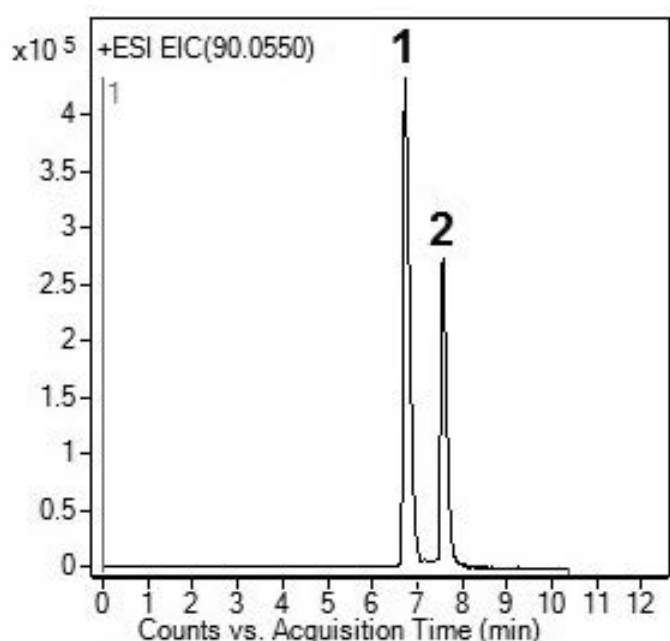

1. Sarcosine



2.  $\beta$ -Alanine

#### Peaks:

1. Sarcosine
2.  $\beta$ -Alanine

### Method Conditions

**Column:** Cogent Diamond Hydride™, 4 $\mu$ m, 100Å

**Catalog No.:** 70000-15P-2

**Dimensions:** 2.1 x 15mm

**Mobile Phase:**

A: 50% Isopropyl Alcohol / 50% DI Water / 0.1% Acetic Acid

Printed from the Chrom Resource Center

Copyright 2024, All Rights Apply

**MicroSolv Technology Corporation**

9158 Industrial Blvd. NE, Leland, NC 28451

tel. (732) 380-8900, fax (910) 769-9435

Email: customers@mtc-usa.com

Website: www.mtc-usa.com

B: 97% Acetonitrile / 3% DI Water / 0.1% Acetic Acid

**Gradient:**

| Time (minutes) | %B |
|----------------|----|
| 0              | 75 |
| 3              | 75 |
| 4              | 65 |
| 5              | 65 |
| 10             | 20 |
| 12             | 75 |

**Temperature:** 50°C

**Post Time:** 5 minutes

**Flow rate:** 0.6mL / minute

**Detection:** ESI - POS - Agilent 6210 MSD TOF Mass Spectrometer

**Injection vol.:** 1µL

**Sample Preparation:** 10mg / L each of Sarcosine and Beta-Alanine in 50:50 A:B

**Note:** When Reversed Phase Columns were evaluated for their ability to separate Sarcosine from Beta-Alanine, both compounds eluted at the solvent front and were not separated. To achieve separation, a very intensive sample preparation has to be employed (e.g. derivatization) when using RP methods.



**Attachment**

**No 129 Sarcosine Analyzed with LCMS pdf** 0.2 Mb [Download File](#)

Printed from the Chrom Resource Center

Copyright 2024, All Rights Apply

**MicroSolv Technology Corporation**

9158 Industrial Blvd. NE, Leland, NC 28451

tel. (732) 380-8900, fax (910) 769-9435

Email: [customers@mtc-usa.com](mailto:customers@mtc-usa.com)

Website: [www.mtc-usa.com](http://www.mtc-usa.com)