
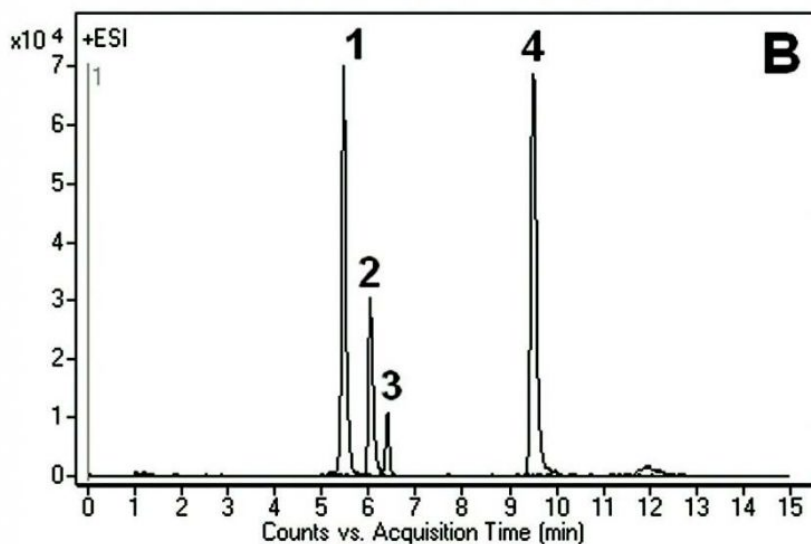


Domoic Acid, Amino Acids, & Ornithine Analyzed with LCMS - AppNote

LC-MS Analysis without Analyte Derivatization

The potent toxin, Domoic Acid is a highly polar compound which is poorly retained on most Reversed Phase Columns. In this Method, not only was Domoic Acid well Retained but also two isobaric compounds (L-Asparagine and Ornithine) were Retained and Separated. In addition, the Peak obtained for Aspartic Acid was very Symmetrical. From these chromatograms, it is clear that the two cell extracts show differences in the ratios between the analyzed compounds (Figure A vs. B).

The presented Method can be used in studies of cell extracts. In addition, it is Robust and Reproducible. The Column in this Method requires a very short Equilibration time between Gradient runs and the Method does not require pre-Column derivatization of any of the analytes.

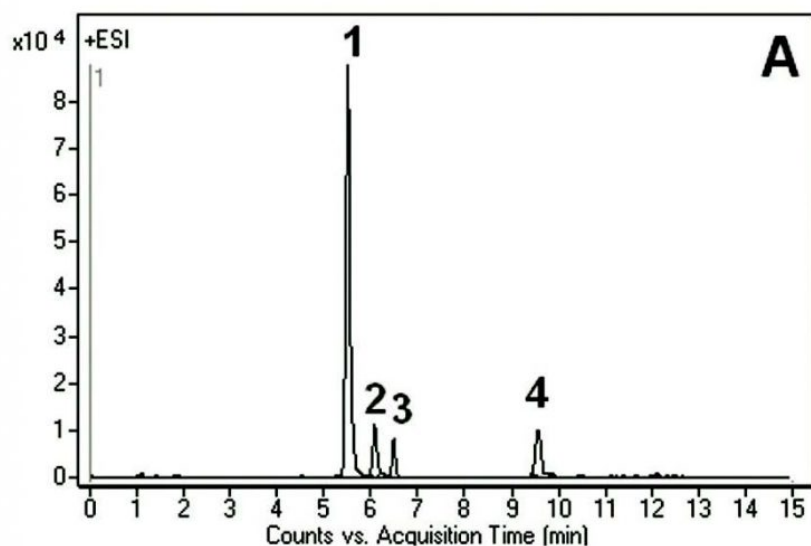

Printed from the Chrom Resource Center

Copyright 2024, All Rights Apply


MicroSolv Technology Corporation

9158 Industrial Blvd. NE, Leland, NC 28451

tel. (732) 380-8900, fax (910) 769-9435

Email: customers@mtc-usa.com

Website: www.mtc-usa.com

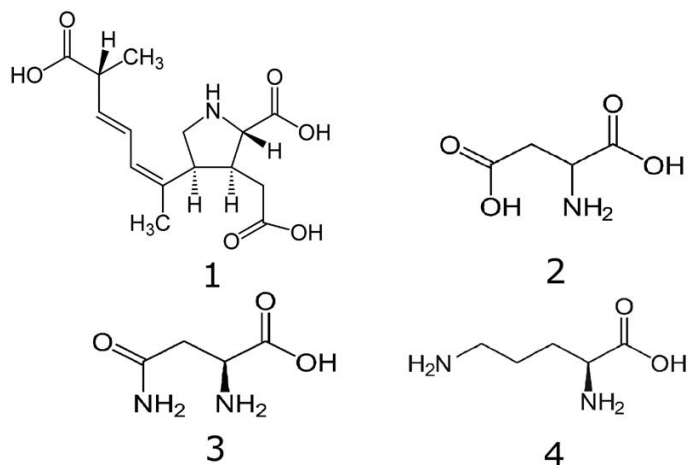

Peaks:

1. Domoic Acid 312.1442 m/z (M+H)⁺
2. L-aspartic Acid 134.0453 m/z (M+H)⁺
3. L-asparagine 133.0608 m/z (M+H)⁺
4. Ornithine 133.0972 m/z (M+H)⁺

Method Conditions

Column: Cogent Diamond Hydride™, 4μm, 100Å

Catalog No.: 70000-15P-2

Dimensions: 2.1 x 150mm

Mobile Phase:

A: 50% DI Water / 50% Methanol / 0.1% Formic Acid

B: Acetonitrile / 0.1% Formic Acid

Gradient:

Time (minutes)	%B
0	95
7	20
10	20
11	95

Post Time: 5 minutes

Injection vol.: 1μL

Flow rate: 0.4mL / minute

Detection: ESI - POS - Agilent 6210 MSD TOF Mass Spectrometer

Sample Preparation: Methanolic extracts of proprietary cell cultures A and B, isolated by filtration.

t₀: 0.9 minutes

Note: Domoic Acid, a compound known for some 30 years, was found to have neurotoxic effects on humans. Upon ingestion, it causes diarrhea, dizziness, seizures, permanent brain damage, and sometimes death.

Printed from the Chrom Resource Center

Copyright 2024, All Rights Apply

MicroSolv Technology Corporation

9155 Industrial Blvd, NE, Raleigh, NC 28451

tel. (732) 380-8900, fax (910) 769-9435

Email: customers@mtc-usa.com

Website: www.mtc-usa.com

Attachment

No 153 Domoic Acid, Amino Acids, & Ornithine Analyzed with LCMS pdf 0.4 Mb [Download File](#)

Printed from the Chrom Resource Center

Copyright 2024, All Rights Apply

MicroSolv Technology Corporation

9158 Industrial Blvd. NE, Leland, NC 28451

tel. (732) 380-8900, fax (910) 769-9435

Email: customers@mtc-usa.com

Website: www.mtc-usa.com