
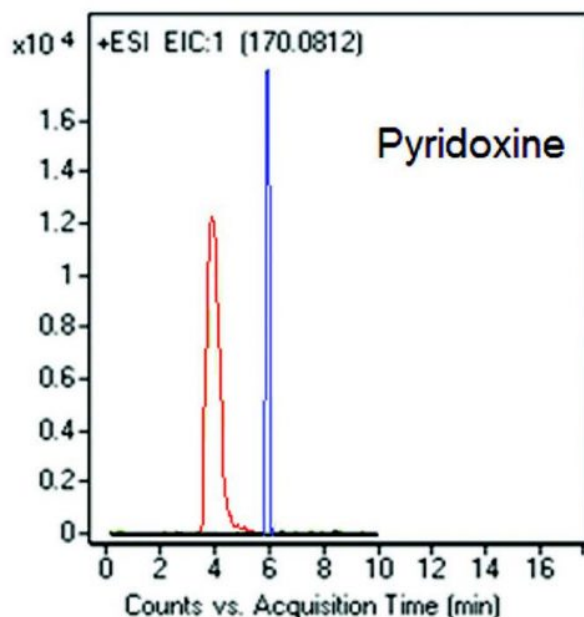




Hydrophilic Vitamins Analyzed with LCMS – AppNote

Different Mobile Phase for LCMS from a UV Method was Needed

Hydrophilic Vitamin analyses were developed using UV detection. However, when the same Method and Mobile Phase was tried with MS Detection, the Peak intensities were very low and Peak Shape for Pyridoxine was not acceptable (see Red Peaks in Figures below).

The Mobile Phase was changed and did not include Ammonium Formate since Positive Mode of Ionization was used with the MS. The Peaks (see Blue Peaks in Figures), were much more Symmetrical, well Separated from each other and Peak intensities were much higher. pH should always be considered when transferring methods from UV to LCMS.

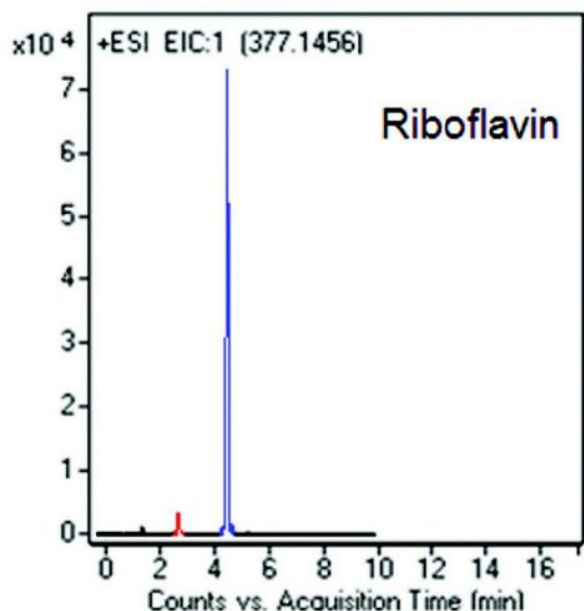

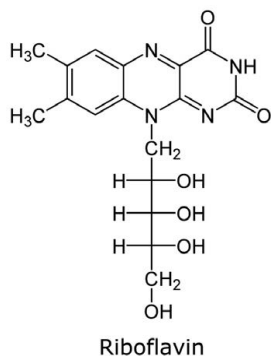

Peaks:

Riboflavin 377.1456 m/z [M+H]⁺

Pyridoxine 170.0812 m/z [M+H]⁺

Method Conditions

Column: Cogent Diamond Hydride™, 4µm, 100Å

Catalog No.: 70000-15P-2

Dimensions: 2.1 x 150mm

Mobile Phases:

For Red Peaks

A: DI Water with 10mM Ammonium Formate / 0.05% Formic Acid (pH 3.5)

B: 95:5 Acetonitrile / 10mM Ammonium Formate (w/v pH 6.5)

For Blue Peaks

A: 50:50 DI Water / 2-Propanol with 0.1% Formic Acid

B: Acetonitrile with 0.1% Formic Acid

Gradient:

Time (minutes)	%B
0	95
1.5	95
4	30
5	30
6	30
7	95

Post Time: 3 minutes

Injection vol.: 1µL

Flow rate: 0.4mL / minute

Detection: ESI - POS - Agilent 6210 MSD TOF Mass Spectrometer

Samples:

Stock Solution: Riboflavin 5mg / L and Pyridoxine 100mg / L in 50:50 Solvent A / Solvent B. The solution was filtered through a 0.45µm Syringe Filter (MicroSolv Tech Corp.).

Samples for Injection were diluted 1:100 with 50:50 Solvent A:B mixture.

Printed from the Chrom Resource Center

Copyright 2024, All Rights Apply

MicroSolv Technology Corporation

9158 Industrial Blvd. NE, Leland, NC 28451

tel. (732) 380-8900, fax (910) 769-9435

Email: customers@mtc-usa.com

Website: www.mtc-usa.com

t₀: 0.9 minutes

Note: Riboflavin and Pyridoxine are two types of B Vitamins and are shown in two different Chromatograms above. These compounds are hydrophilic and hence may be difficult to retain by conventional Reversed Phase Methods.



Attachment

No 244 Hydrophilic Vitamins Analyzed with LCMS pdf 0.4 Mb [Download File](#)

Printed from the Chrom Resource Center

Copyright 2024, All Rights Apply

MicroSolv Technology Corporation

9158 Industrial Blvd. NE, Leland, NC 28451

tel. (732) 380-8900, fax (910) 769-9435

Email: customers@mtc-usa.com

Website: www.mtc-usa.com