


Atorvastatin HPLC Method Transfer to UHPLC – AppNote


Transfer to “near-UHPLC” 2.2µm Column, for the API Atorvastatin

This Application Note demonstrates how data obtained on a 4µm Cogent Bidentate C18 Column (*Figure B*) can be adapted for a 2.2µm Column (*Figure A*). The retention times of both analytes are very comparable in each figure. This Method produces excellent Separation of the API and its main acid degradant and is LCMS compatible which can be used in clinical applications involving plasma samples.

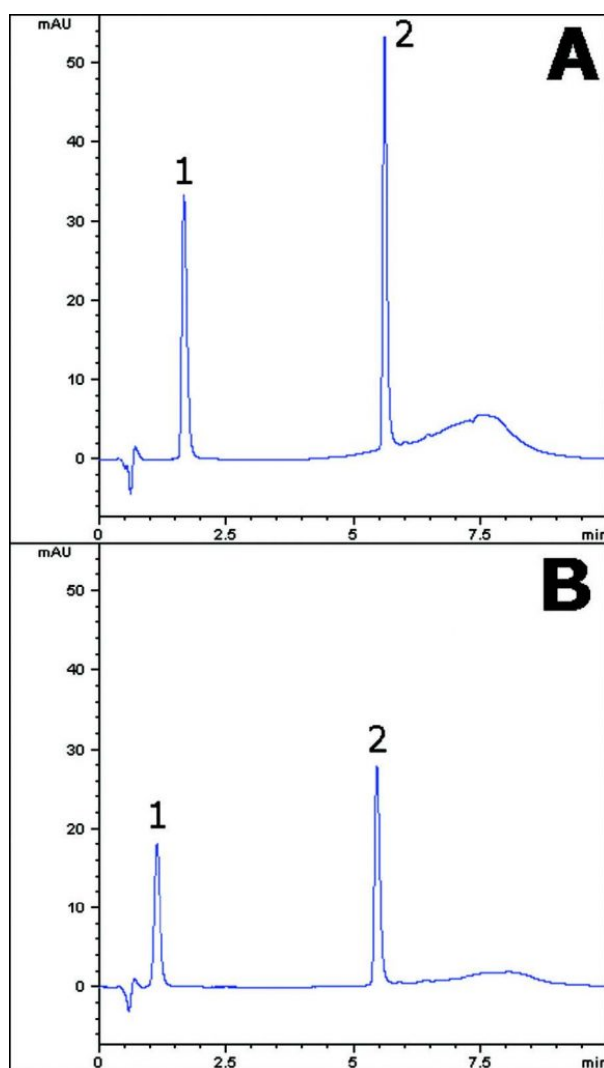

Peaks:

1. Atorvastatin
2. Atorvastatin Lactone

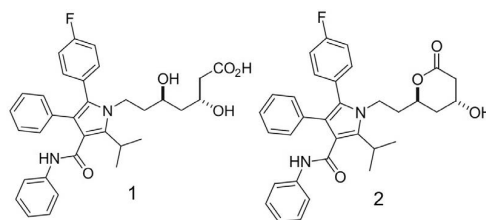

Method Conditions

Columns:

Figure A: Cogent Bidentate C18 2.0™, 2.2µm, 120Å

Figure B: Cogent Bidentate C18™, 4µm, 100Å

Catalog Nos.:

Printed from the Chrom Resource Center

Copyright 2024, All Rights Apply

MicroSolv Technology Corporation

9158 Industrial Blvd. NE, Leland, NC 28451

tel. (732) 380-8900, fax (910) 769-9435

Email: customers@mtc-usa.com

Website: www.mtc-usa.com

Figure A: [40218-05P-2](#)

Figure B: [40018-05P-2](#)

Column Dimensions: 2.1 x 50mm

Mobile Phases:

A: DI Water / 10mM Ammonium Acetate

B: 90:10 Acetonitrile / DI Water / 10mM Ammonium Acetate

Gradients:

Time (minutes)	%B
0	40
1	100
6	100
7	40

Flow rates: 0.3mL / minute

Detection: UV @ 248nm

Sample Preparation: 40mg strength Lipitor® tablet (Atorvastatin) was ground and added to a 50mL volumetric flask with a portion of Solvent B diluent. The solution was sonicated 10 minutes and diluted to mark with Solvent B. It was then filtered through a 0.45µm Nylon Syringe Filter (MicroSolv Tech Corp.). The filtrate was diluted 4x in a diluent of 50:50 Solvent B / 1N HCL. It was heated in a dry bath for 10 minutes at 85°C.



Attachment

No 308 Atorvastatin HPLC Method Transfer to UHPLC pdf 0.4 Mb [Download File](#)

Printed from the Chrom Resource Center

Copyright 2024, All Rights Apply

MicroSolv Technology Corporation

9158 Industrial Blvd. NE, Leland, NC 28451

tel. (732) 380-8900, fax (910) 769-9435

Email: customers@mtc-usa.com

Website: www.mtc-usa.com