


## Neomycin Sulfate Analyzed with LCMS - AppNote

Neomycin presents a number of challenges to routine Chromatographic Analysis. It lacks Chromophores and therefore is difficult to detect using conventional HPLC techniques and retention in traditional Reversed Phase mode may not be viable due to its high polarity. However, use of the Cogent Diamond Hydride Column in conjunction with a Mass Spec helps circumvent these issues. The presented data illustrates how the Compound can be both readily retained, with good run-to-run precision, and adequately detected using Mass Spectrometry.

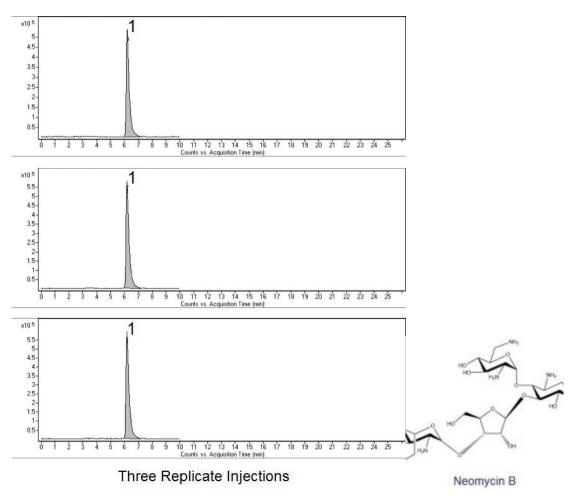

Peak:

Neomycin 615.3196 n/z (M+H)+

## **Method Conditions:**

Gradient:

Column: Cogent Diamond Hydride<sup>™</sup>, 4µm, 100Å
Catalog No.: 70000-05P-2
Dimensions: 2.1 x 50 mm
Mobile Phase:

A: DI Water / 0.1% Formic Acid
B: Acetonitrile / 0.1% Formic Acid

Printed from the Chrom Resource Center Copyright 2024, All Rights Apply **MicroSolv Technology Corporation** 9158 Industrial Blvd. NE, Leland, NC 28451 tel. (732) 380-8900, fax (910) 769-9435 Email: customers@mtc-usa.com Website: www.mtc-usa.com

## MICROS

%B
90
90
10
10
90
90

Injection Volume: 5µL

Flow Rate: 0.3 mL/minute

**Detection**: ESI – POS – Agilent 6210 MSD TOF Mass Spectrometer

Sample Preparation: 0.1 mg/mL Neomycin Sulfate Reference Standard Solution in Solvent A Diluent

**Note:** Neomycin is aminoglycoside compound that is used as an antibiotic in various types of topical formulations. It is a component of the popular topical cream Neosporin<sup>®</sup>, used to pre-vent infections. It was discovered by biochemist and microbiologist Selman Waksman and colleagues.



Attachment

No 372 Neomyin sulfate.pdf 0.2 Mb Download File

Printed from the Chrom Resource Center Copyright 2024, All Rights Apply **MicroSolv Technology Corporation** 9158 Industrial Blvd. NE, Leland, NC 28451 tel. (732) 380-8900, fax (910) 769-9435 Email: customers@mtc-usa.com Website: www.mtc-usa.com