
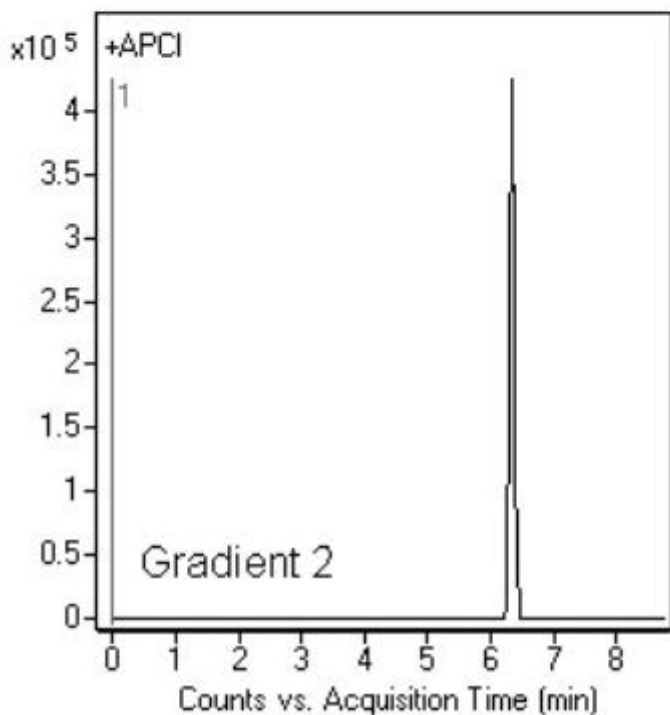



Simple and easy prednisone analysis with LCMS detection

This method does not require any type of derivatization. Two Gradients are presented which will allow you to choose one depending on other components in the sample and your Method objectives. Retention can be achieved on a very short column (50 mm) as shown. Linear gradient conditions were used for analysis of this important Corticosteroid.

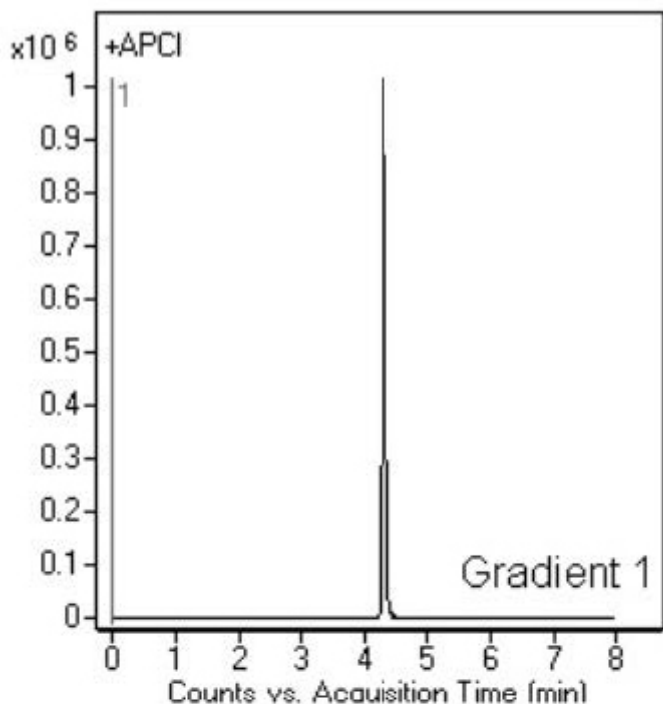

Peak:

Prednisone 359.1853 m/z (M+H)⁺

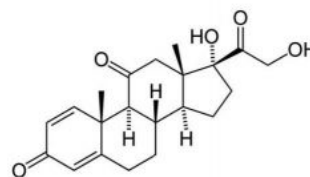

Prednisone

Source Center
Rights Apply

MicroSolv Technology Corporation

9158 Industrial Blvd. NE, Leland, NC 28451
tel. (732) 380-8900, fax (910) 769-9435

Email: customers@mtc-usa.com

Website: www.mtc-usa.com

Method Conditions

Column: Cogent Bidentate C18™, 4µm, 100Å

Catalog No.: 40018-05P-2

Dimensions: 2.1 x 50 mm

Mobile Phase:

A: DI Water+ 0.1% Formic Acid

B: Methanol + 0.1% Formic Acid

Gradient 1:

Time (minutes)	%B
0	10
5	100
7	100
8	10

Gradient 2:

Time (minutes)	%B
0	10
10	100
11	100
12	10

Post Time: 5 minutes

Total Time: 12 minutes

Injection vol.: 1µL

Flow rate: 0.4mL / minute

Detection: APCI - POS - Agilent 6210 MSD TOF Mass Spectrometer

Sample Preparation: Prednisone 100ng / mL prepared in 100% B and diluted 1:10 before analysis

Note: The administration of Prednisone, a synthetic analog of Cortisone, suppresses production of Cortisol and monitoring the concentration of this Corticosteroid has significant therapeutic and clinical importance. Prednisone and Prednisolone were introduced by Schering Corporation in the mid-1960s under the brand names Meticorten® and Meticortelone®, respectively. These prescription medicines are now available from a number of manufacturers as generic drugs.



Attachment

Quantitation of Prednisone with LCMS pdf

Printed from the Chrom Resource Center

Copyright 2024, All Rights Apply

MicroSolv Technology Corporation

9158 Industrial Blvd. NE, Leland, NC 28451

tel. (732) 380-8900, fax (910) 769-9435

Email: customers@mtc-usa.com

Website: www.mtc-usa.com