



Determination of Atropine by HPLC – AppNote

Rugged & Fast Without Paired Ion Reagents

Ion-pair Chromatography (IPC) is commonly used in order to retain Atropine on ordinary Reversed Phase HPLC Columns. Beside long equilibration times with these columns, IPC often suffers from poor robustness.

Using an isocratic elution with flow rate 1 mL / minutes gave symmetrical peak for this Tropane Alkaloid. The sensitivity is sufficient for the proper determination of Atropine in plasma after intravenous administration of the drug to hospitalized patients.

This method is also useful for testing for drug poisoning and for stability testing of Atropine solutions during manufacturing. The linear range of detection for Atropine was around 5.0 µg / mL with a limit of quantification (LOQ) 10.0 µg / mL.

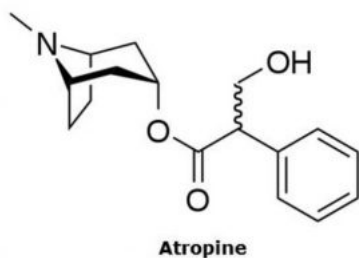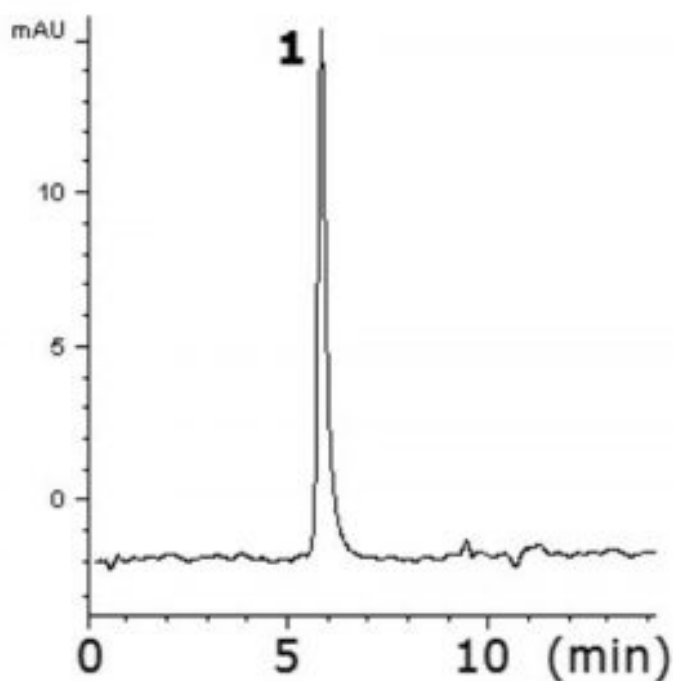

Peak:

Atropine (RT = 5.94 min)

Method Conditions

Column: Cogent UDC-Cholesterol™, 4µm, 100Å

Catalog No.: [69069-15P](#)

Dimensions: 4.6 x 150mm

Mobile Phase:

A: DI Water + 0.1% Acetic Acid + 0.005% TFA

B: Acetonitrile + 0.1% Acetic Acid + 0.005% TFA

Flow rate: 1mL / minute

Detection: UV @ 214nm

Injection vol.: 1µL

Sample Preparation: Prepared in 50% Solution A / 50% Solution B, concentration 1mg / mL Sample was filtered through a 0.45µm Nylon Syringe Filter prior to HPLC-UV injections (MicroSolv Technology Corp.)

Note: Being potentially deadly, Atropine derives its name from Atropos, one of the three Fates who, according to Greek mythology, chose how a person was to die. Atropine is a core medicine in the World Health Organization's "Essential Drugs List", which is a list of minimum medical needs for a basic health care system.



Attachment

No 119 Determination of Atropine by HPLC pdf 0.1 Mb [Download File](#)

Printed from the Chrom Resource Center

MicroSolv Technology Corporation

9158 Industrial Blvd. NE, Leland, NC 28451

tel. (732) 380-8900, fax (910) 769-9435

Email: customers@mtc-usa.com

Website: www.mtc-usa.com

Date: 05-05-2024