
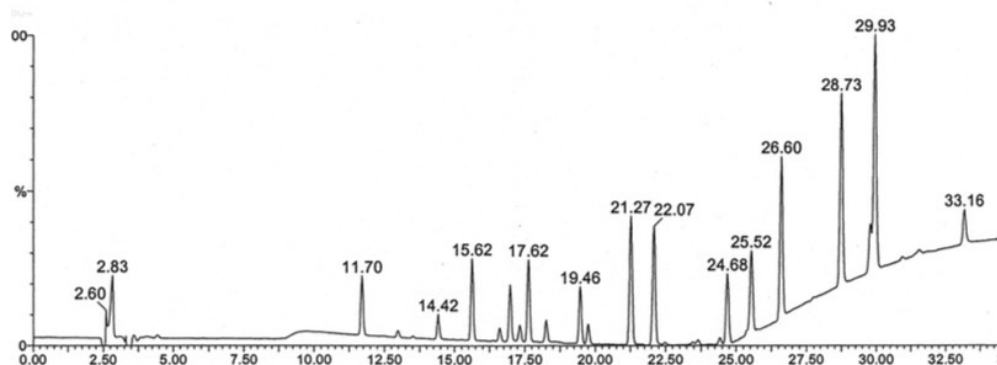
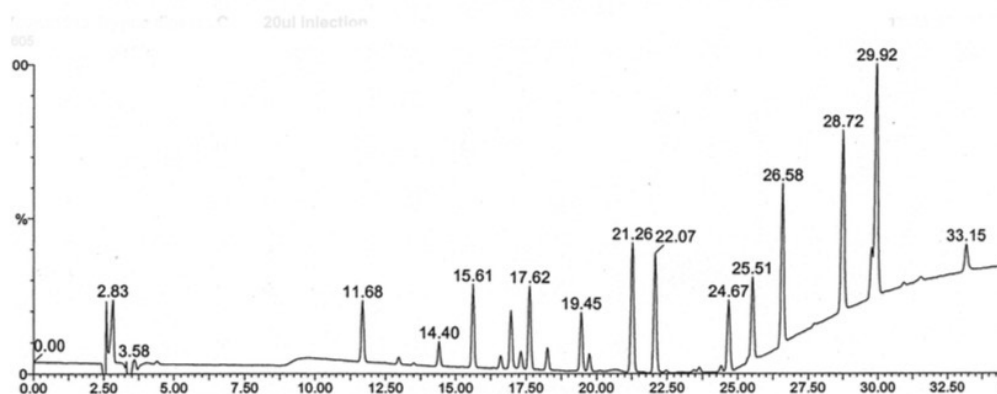


## Synthetic Peptide Analyzed with HPLC - AppNote

### Peptide Production Confirmation Using the Cogent HPS® C18

An in-process Method for Qualifying a synthetic peptide is shown with 3 samples of tryptic “digests” were injected on the same Column. The Reproducibility from run to run on the samples is excellent giving the user a high level of confidence. The process and Method was further confirmed by coupling the HPLC Separation directory to Mass Spectrometry. The Mass data had a high degree of Accuracy and Reproducibility, verifying the peptide.

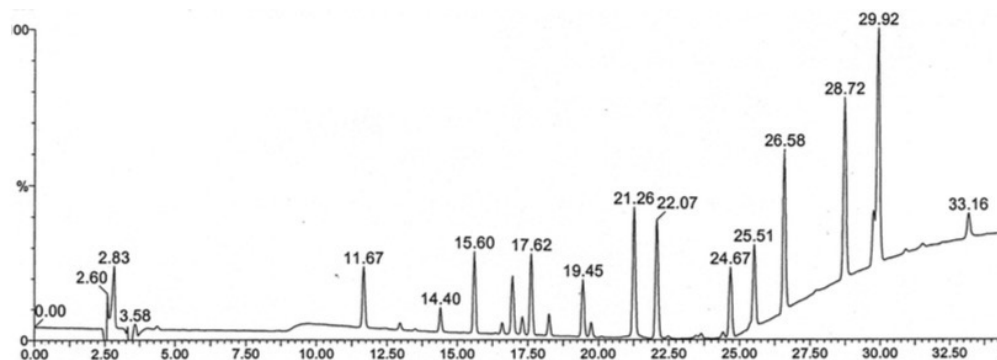

### Method Conditions

**Column:** Cogent HPS C18™, 5µm, 120Å

**Catalog No.:** 75018-25P

**Dimensions:** 4.6 x 250mm

**Mobile Phase:**

A: DI Water with 0.1% Trifluoroacetic Acid (TFA)

B: Acetonitrile with 0.1% Trifluoroacetic Acid (TFA)

**Gradient:**

Time (minutes)	%B
0	0
20	60
20.1	0

**Temperature:** 30°C

**Injection vol.:** 20µL

**Flow rate:** 1mL / minute

**Detection:** UV @ 254nm

**Sample Preparation:** 3 Different Samples from the same peptide batch were digested using Trypsin and injected onto the HPLC Column.

**Notes:** *Cogent HPS C18 Columns are perfectly suited for peptide analysis. The pore diameter, the exhaustive end capping and the low metal content of the Silica make these Columns an excellent choice for Peptide Mapping after digestion with Trypsin also known as a Tryptic Digest. Unique Selectivity and low cost make these Columns the choice of many Protein laboratories worldwide when Reproducibility and Reliability are mandatory.*



**Attachment**

**No 16 Synthetic Peptide Production.pdf** 0.2 Mb [Download File](#)

Printed from the Chrom Resource Center

**MicroSolv Technology Corporation**

9158 Industrial Blvd. NE, Leland, NC 28451

tel. (732) 380-8900, fax (910) 769-9435

Email: [customers@mtc-usa.com](mailto:customers@mtc-usa.com)

Website: [www.mtc-usa.com](http://www.mtc-usa.com)

Date: 07-27-2024