
# MICROS

### Furazolidone Analyzed by HPLC - AppNote


#### **Improved Specificity Compared to USP Assay Method**

The USP Assay Method for Furazolidone is performed by UV Spectrophotometry. This HPLC Method provides more Robustness and Specificity for the analysis. Separation of Furazolidone from the structurally similar compound Nitrofurantoin is shown in the figure.

Nitrofurantoin can be used as an internal standard to obtain more robust Quantitation. Furthermore, the ability of this Method to distinguish amongst similar compounds demonstrates how it is less prone to interference from impurities or degradants. Two Chromatograms are overlayed to present the precision of the Method using two different Columns made from different lots.

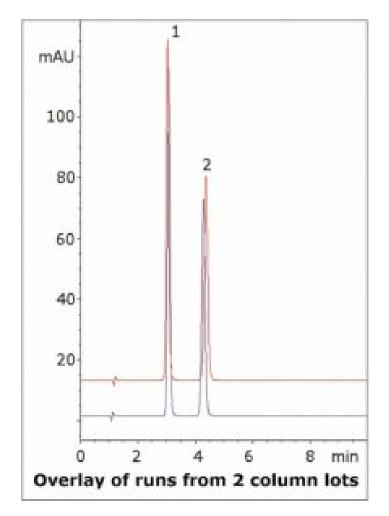

## MICROS



1. Nitrofurantoin (Internal Standard) 2. Furazolidone

#### **Method Conditions**

Column: Cogent Bidentate C8<sup>™</sup>, 4µm, 100Å
Catalog No.: 40008-75P
Dimensions: 4.6 x 75mm
Mobile Phase: 80% DI Water / 20% Acetonitrile / 0.1% Formic Acid (v/v)
Injection vol.: 1µL
Flow rate: 1.0mL / minute
Detection: UV @ 367nm
Sample Preparation: 1mg Furazolidone and 1mg Nitrofurantoin USP reference standards were dissolved in 1mL of the Mobile Phase. The solution was then diluted 1:10 with the same diluent. Peak identities were confirmed with individual standards.

to: 0.9 minutes

**Note:** Furazolidone is an antibacterial Nitrofuran. It is used in both human and veterinary medicine. It is available under the trade name Furoxone<sup>®</sup>.



Attachment

No 205 Furazolidone Analyzed by HPLC pdf 0.6 Mb Download File

Printed from the Chrom Resource Center **MicroSolv Technology Corporation** 9158 Industrial Blvd. NE, Leland, NC 28451 tel. (732) 380-8900, fax (910) 769-9435 Email: customers@mtc-usa.com Website: www.mtc-usa.com Date: 04-05-2024