
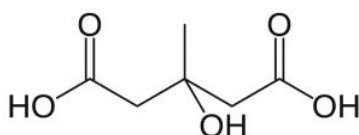


Important Biomarker for Diabetes and HMG Disorder is well retained by HPLC.

A selective, specific, and sensitive HPLC method with LCMS Analysis has been developed for the determination of 3-hydroxy-3-methylglutaric acid (a.k.a. Meglutol) in urine samples. The method can be also used in the analysis of plasma samples after precipitation of plasma proteins with Acetonitrile. The retention was achieved using a Cogent Diamond Hydride Column.

This method can be used for screening of large numbers of urine or Plasma Samples, due to simple Sample Preparation and Rapid Equilibration of the Column even when gradient analysis is used.

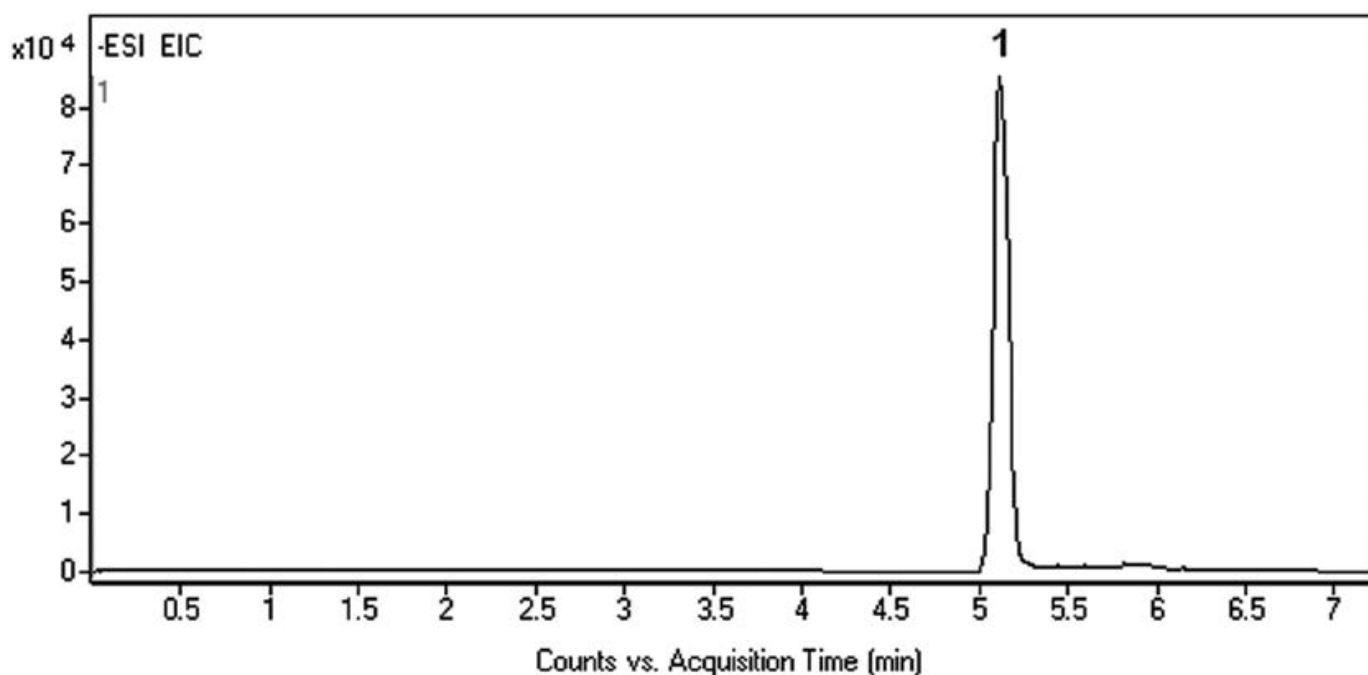

Meglutol

Peak:

3-hydroxy-3-methylglutaric acid 161.0455 m/z [M-H]⁻

Method Conditions

Column: Cogent Diamond Hydride™, 4μm, 100Å

Catalog No.: 70000-15P-2

Dimensions: 2.1 x 150 mm

Mobile Phase:

A: DI H₂O / 10 mM Ammonium Formate

B: 95% Acetonitrile / 5% DI Water / 10 mM Ammonium Formate (v/v)

Gradient:

Time (minutes)	%B
----------------	----

Printed from the Chrom Resource Center

Copyright 2024, All Rights Apply

MicroSolv Technology Corporation

9158 Industrial Blvd. NE, Leland, NC 28451

tel. (732) 380-8900, fax (910) 769-9435

Email: customers@mtc-usa.com

Website: www.mtc-usa.com

0	95
1	95
5	30
7	30
8	95

Post Time: 3 minutes

Injection vol.: 1 μ L

Flow rate: 0.4 mL/minute

Detection: ESI - NEG - Agilent 6210 MSD TOF Mass Spectrometer

t₀: 0.9 minutes

Note: When a set of plasma samples were analyzed, the concentrations of 3-hydroxy-3-methylglutaric acid were significantly higher in diabetic patients than those of healthy controls. For this reason it was important to develop a reliable Analytical Method for the analysis of this Compound. The increased level in urine of this metabolite is also observed in an inborn disease 3-hydroxy-3-methylglutaric Aciduria. Early detection is crucial for successful treatment.



Attachment

No 233 3-Hydroxy-3-Methylglutaric acid HMG in Urine.pdf 0.2 Mb [Download File](#)

Printed from the Chrom Resource Center

Copyright 2024, All Rights Apply

MicroSolv Technology Corporation

9158 Industrial Blvd. NE, Leland, NC 28451

tel. (732) 380-8900, fax (910) 769-9435

Email: customers@mtc-usa.com

Website: www.mtc-usa.com