


# Barbiturates Analyzed with LCMS - AppNote

# Standard Solutions in Human Urine Spiked with Barbiturates

After minimal sample preparation (*dilute-and-shoot approach*), spiked urine samples were analyzed using a C18 Column. The analysis was based on a Separation of Standards [1]. The obtained Peaks were Symmetrical (As<1.05) and Efficient (> 106 pl/m). No shift in retention Times was observed after the samples were diluted ten-fold (*data not shown*). Matrix effects that would diminish the signal intensity were less than 5%.

This Method shows a possible Application for Analysis of these Compounds in Forensic Samples.

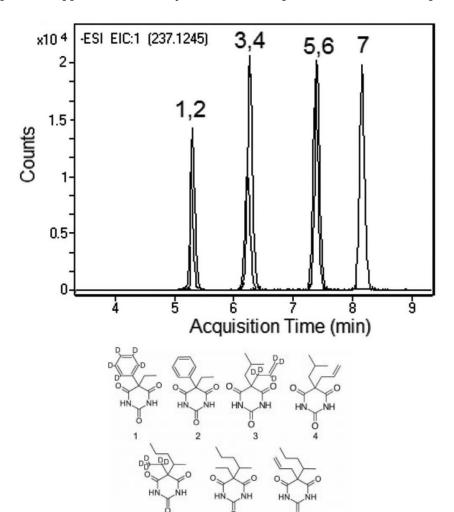

Peaks:

- 1. Phenobarbital-D5 m/z = 236.1089,
  - 2. Phenobarbital m/z = 231.0775,
  - 3. Butalbital-D5 m/z = 228.1402,
    - 4. Butalbital m/z = 223.1088,
- 5. Pentobarbital-D5 m/z = 230.1558,
  - 6. Pentobarbital m/z = 225.1245,
  - 7. Secobarbital m/z = 237.1245



## **Method Conditions**

Column: Cogent Bidentate C18<sup>™</sup>, 4µm, 100Å

**Catalog No.**: 40018-05P-2 **Dimensions**: 2.1 x 50mm

**Mobile Phase:** 

A: DI Water with 10mM Ammonium Formate

B: 95:5 Acetonitrile / DI Water with 10mM Ammonium Formate (v/v)

### **Gradient**:

Time (minutes)	%B
0	10
1	10
10	45

Post Time: 3 minutes
Injection vol.: 1µL

Flow rate: 0.4mL / minute

Detection: ESI - NEG - Agilent 6210 MSD TOF Mass Spectrometer

**Sample Preparation**: Stock solutions of Barbiturates were prepared at a concentration of 1mg / mL in Methanol. Then 2mL of a urine sample was spiked with the stock solutions diluted, (dilution 1:100) and filtered through a 0.45µm Nylon Syringe Filter (MicroSolv Tech Corp.) into Autosampler Vials.

**to**: 0.3 minutes



[1] J.J.Pesek, M.T. Matyska, A.M. Kim, J. Sep. Sci. 2013, 36, 2760-2766.

#### **Attachment**

No 270 Barbiturates Analyzed with LCMS pdf 0.3 Mb Download File

Printed from the Chrom Resource Center

**MicroSolv Technology Corporation** 

9158 Industrial Blvd. NE, Leland, NC 28451 tel. (732) 380-8900, fax (910) 769-9435

Email: customers@mtc-usa.com

Website: www.mtc-usa.com

Date: 05-16-2024