


Ocella® Tablet Analyzed with HPLC - AppNote

Separation of Drospirenone and Ethinyl Estradiol


Good Selectivity with high Efficiency Peaks can be achieved analyzing Ocella Tablets. This can be helpful since Ethinyl Estradiol is present at a much lower concentration than Drospirenone and therefore can be difficult to detect; the high Efficiency can contribute to a stronger Signal in detection thus increasing Sensitivity. Furthermore, the isocratic Mobile Phase is very simple to prepare or even obtain pre-mixed, allowing for streamlined routine Assays of this formulation in QC laboratories.

Figure A shows the full view of the Chromatogram, with the Drospirenone Peak shown in its entirety. Figure B shows a zoom-in view so that the tiny Ethinyl Estradiol Peak can be seen more clearly and measured. There is even an Impurity Peak observed eluting after Drospirenone.

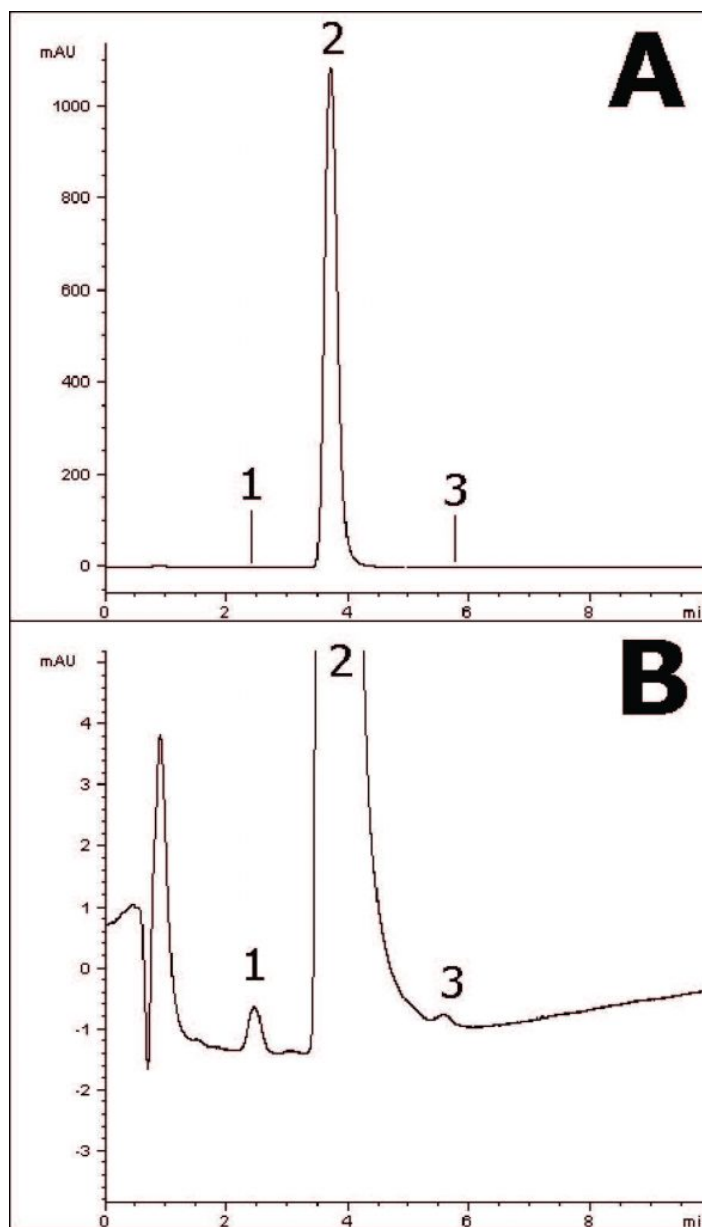

in the Chrom Resource Center
Copyright 2024, All Rights Apply
Solv Technology Corporation
10000 Al Blvd. NE, Leland, NC 28451
380-8900, fax (910) 769-9435
Email: customers@mtc-usa.com

Website: www.mtc-usa.com

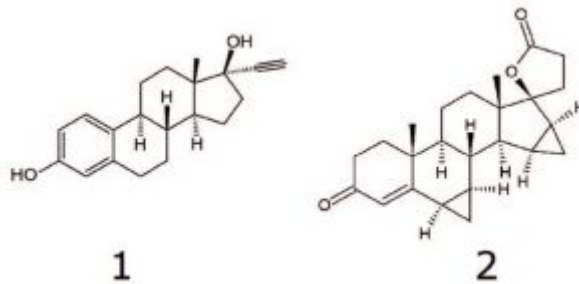

Peaks:

1. Ethinyl estradiol
2. Drospirenone
3. Impurity

Method Conditions

Column: Cogent Bidentate C18 2.0™, 2.2µm, 120Å

Catalog No.: 40218-05P-2

Dimensions: 2.1 x 50mm

Mobile Phase: 50:50 DI Water / Acetonitrile (v/v)

Injection vol.: 4.0µL

Flow rate: 0.2mL / minute

Detection: UV @ 265nm

Sample Preparation: Ocella® Tablet (3mg strength Drospirenone and 0.03mg strength Ethinyl Estradiol) was ground and added to a 10mL volumetric flask containing a portion of Acetonitrile. It was sonicated for 10 minutes and diluted to mark. After mixing, a portion was filtered (0.45µm, Nylon Syringe Filter) and used for HPLC injections.

Note: The combination formulation of Drospirenone and Ethinyl Estradiol is used as a contraceptive and also to alleviate symptoms of premenstrual dysphoric disorder.



Attachment

No 338 Ocella® Tablet Analyzed with HPLC pdf 0.3 Mb [Download File](#)

Printed from the Chrom Resource Center

Copyright 2024, All Rights Apply

MicroSolv Technology Corporation

9158 Industrial Blvd. NE, Leland, NC 28451

tel. (732) 380-8900, fax (910) 769-9435

Email: customers@mtc-usa.com

Website: www.mtc-usa.com