


Pyrilamine & 4-Amino-3-Chloropyridine analysis with HPLC - AppNote

Unique Selectivity on a Cogent Amide Stationary Phase

The Cogent Amide column offers unique selectivity that may not be readily attainable with other phases. Two test solutes shown in this application note (*Pyrilamine* and *4-Amino-3-Chloropyridine*) were baseline separated on the Cogent Amide column (*Figure A*), but they co-eluted with no resolution on a different Cogent column using otherwise equivalent method conditions (*Cogent Diamond Hydride™*, *Figure B*). The presence of the Amide ligand provides additional selectivity that can make a significant difference in resolving closely-eluting compounds such as these.

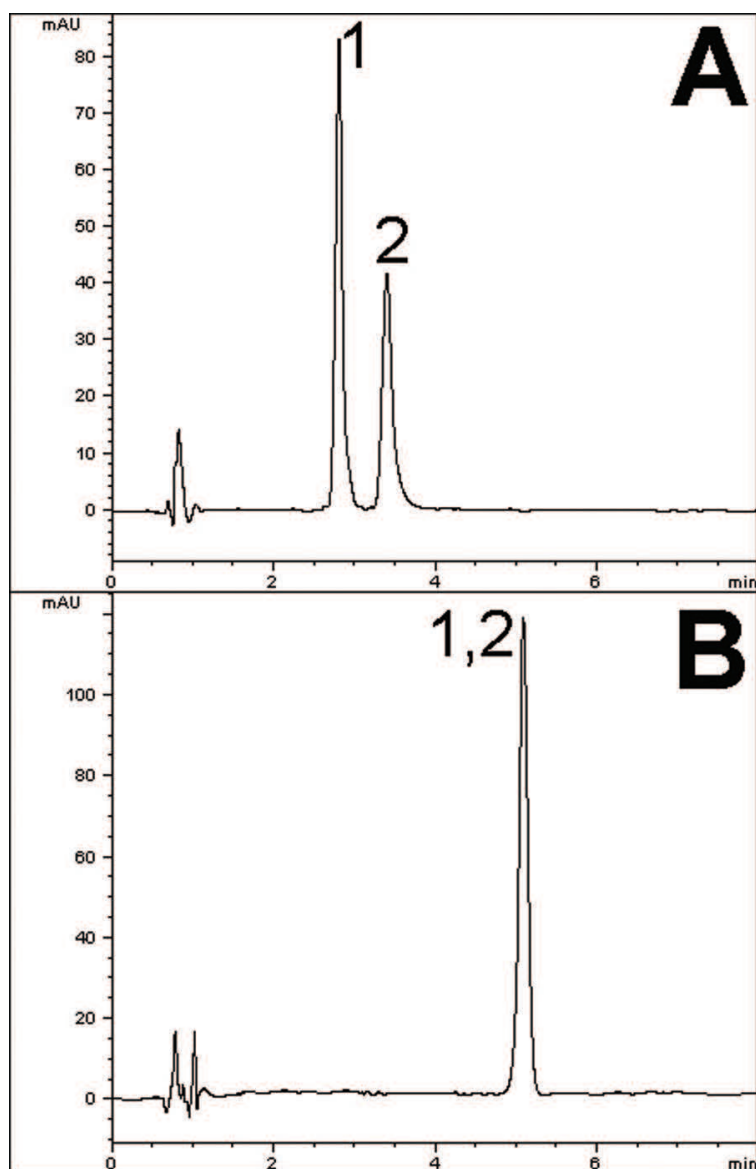

Printed from the Chrom Resource Center

Copyright 2024, All Rights Apply



MicroSolv Technology Corporation

9158 Industrial Blvd. NE, Leland, NC 28451

tel. (732) 380-8900, fax (910) 769-9435

Email: customers@mtc-usa.com

Website: www.mtc-usa.com

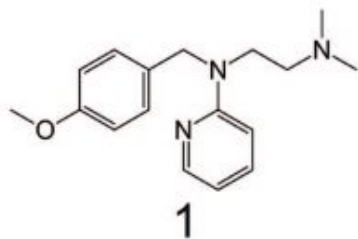

Peaks:

1. Pylamine
2. 4-Amino-3-Chloropyridine

Method Conditions

Column: Cogent Amide™, 4µm, 100Å

Catalog No.: 40036-05P

Dimensions: 4.6 x 50mm

Mobile Phase:

A: 90% DI Water / 10% Acetonitrile / 0.1% Formic Acid (v/v)

B: B: Acetonitrile / 0.1% Formic Acid (v/v)

Gradient:

Time (Minutes)	%B
0	90
1	90
7	50
8	90

Post Time: 3 minutes

Flow rate: 1.0 mL/minute

Detection: UV 244 nm

Injection vol.: 2µL

Sample Preparation:

100 mg/L Pylamine and 4-Amino-3-Chloropyridine reference standards in diluent of 50/50 solvent A/solvent B. Peak identities confirmed with individual standards.

Note: Amine-containing compounds such as Pylamine and 4-Amino-3-Chloropyridine can be difficult to analyze using conventional silica-based stationary phases. These columns have residual silanol groups on the surface that can interact electrostatically with Amines, causing peak tailing. Chromatographers use a number of strategies to avoid these issues, such as use of ion pair agents or endcapping. However, Cogent TYPE-C Silica phases are virtually free of silanols, and therefore good peak shapes can be obtained without these workarounds.

Printed from the Chrom Resource Center

Copyright 2024, All Rights Apply

Attachment

No 352 Ppyrilamine and 4-Amino-3-Chloropyridine.pdf 0.4 Mb [Download File](#)

Printed from the Chrom Resource Center

Copyright 2024, All Rights Apply

MicroSolv Technology Corporation

9158 Industrial Blvd. NE, Leland, NC 28451

tel. (732) 380-8900, fax (910) 769-9435

Email: customers@mtc-usa.com

Website: www.mtc-usa.com