



## Tizanidine HCl Tablet with Precision – AppNote

### Excellent Run to Run Precision

Tizanidine has several amine groups which can present problems to chromatographers. Residual silanols on the surface of ordinary Silica-based Columns can electrostatically interact with these groups, causing peak tailing.

The Cogent Amide Column, used in the Application Note is virtually free of residual silanols and therefore a symmetrical peak shape can be obtained. An overlay of five consecutive runs demonstrates the run- to-run precision when using these columns.

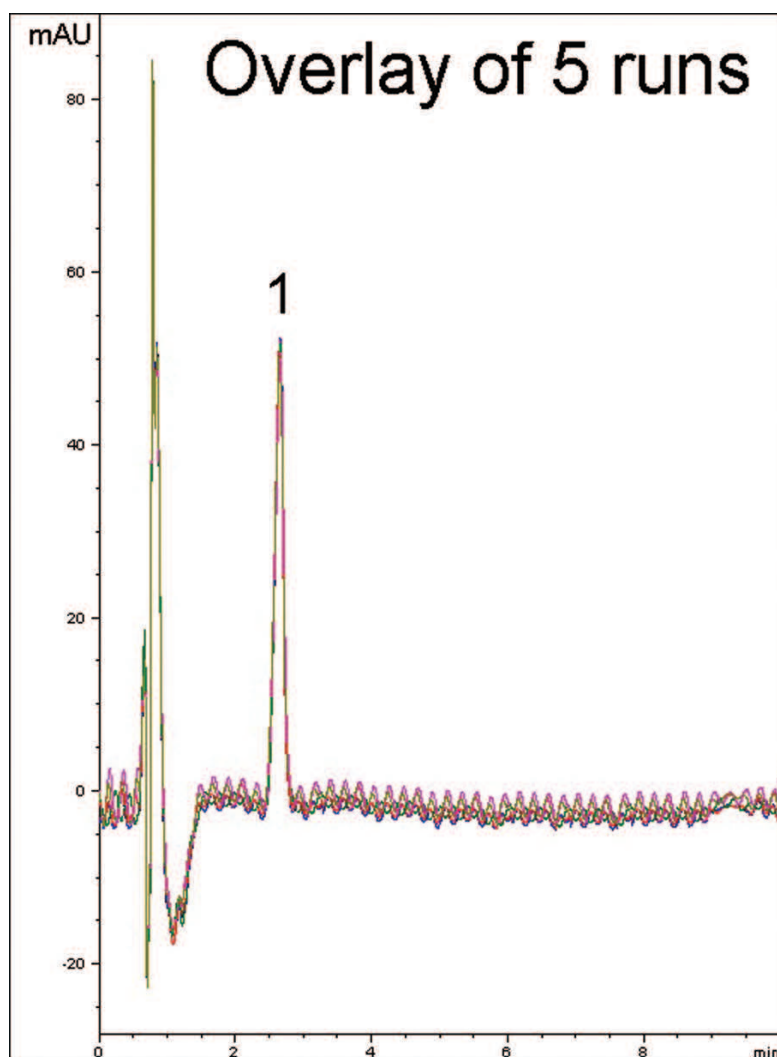

Tizanidine

**Peak:**  
Tizanidine

## Method Conditions

**Column:** Cogent Amide™, 4µm, 100Å

**Catalog No.:** 40036-05P

**Dimensions:** 4.6 x 50mm

### Mobile Phase:

A: 90% DI Water / 10% Acetonitrile / 0.1% Formic Acid (v/v)

B: Acetonitrile / 0.1% Formic Acid (v/v)

### Gradient:

Time (Minutes)	%B
0	90
2	90
6	40
7	90

**Flow rate:** 1.0 mL/minute

**Detection:** UV @ 230nm

**Injection vol.:** 3µL

### Sample Preparation:

4 mg strength Tizanidine HCl tablet was ground and weighed in a 10 mL volumetric flask. A portion of 50/50 solvent A/ solvent B diluent was added and the flask was sonicated 10 minutes. It was then diluted to mark and filtered with a 0.45µm Nylon syringe filter (MicroSolv Tech Corp). An aliquot was then diluted 1:10 with a diluent of 10% solvent A / 90%.

**Note:** Tizanidine is a centrally acting  $\alpha$ 2- adrenergic agonist used to treat spasms, cramping, tightness of muscles, and related conditions. It is available under the trade name Zanaflex® as well as generic versions.



### Attachment

No 356 Tizanidine Amide.pdf 0.5 Mb [Download File](#)

Printed from the Chrom Resource Center  
**MicroSolv Technology Corporation**  
9158 Industrial Blvd. NE, Leland, NC 28451  
tel. (732) 380-8900, fax (910) 769-9435  
Email: [customers@mtc-usa.com](mailto:customers@mtc-usa.com)  
Website: [www.mtc-usa.com](http://www.mtc-usa.com)  
Date: 07-22-2024