


This saw tooth pattern may be due to the presence of an immiscible solvent remaining on the column.

Even trace amounts of these solvents can cause issues. The immiscibility manifests as an unstable baseline, such as the example shown below.

Suggestion: In order to fix this issue, try flushing the column overnight with a mutually miscible solvent such as isopropanol to remove any immiscible non polar solvents that may be in it. This phenomenon can happen to Cogent TYPE-C™ HPLC columns or others that may have been introduced to immiscible solvents. *In some cases, you might observe this with a new column if residual packing solvents may still be present.*

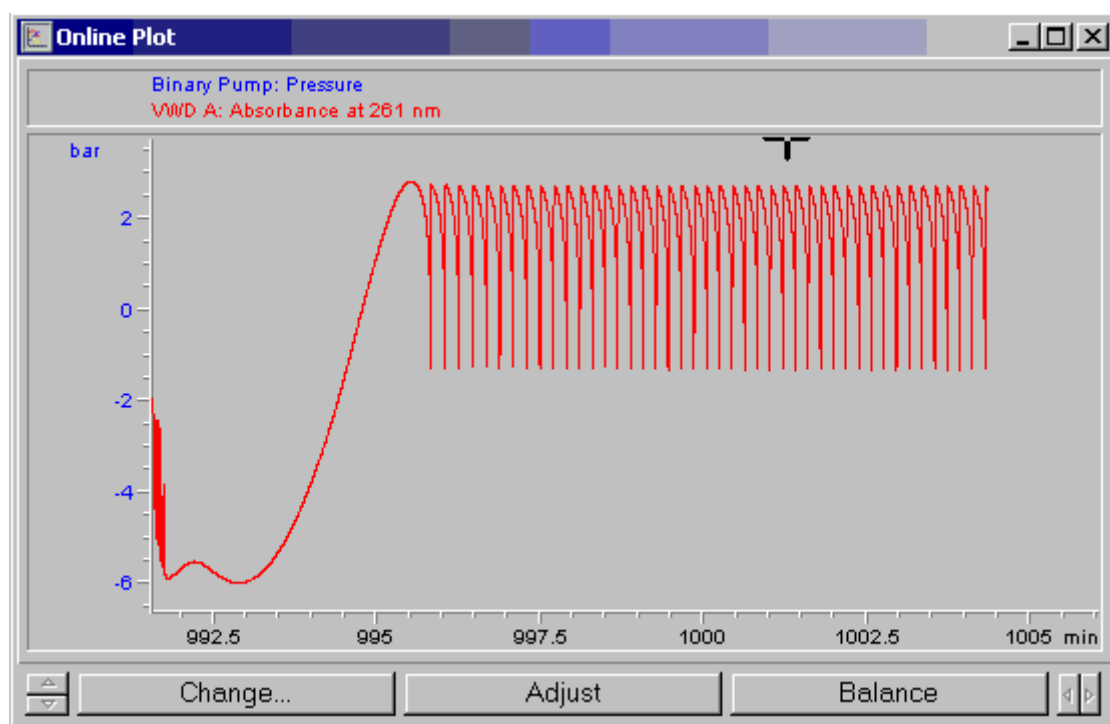

Printed from the Chrom Resource Center

Copyright 2024, All Rights Apply

MicroSolv Technology Corporation

9158 Industrial Blvd. NE, Leland, NC 28451

tel. (732) 380-8900, fax (910) 769-9435

Email: customers@mtc-usa.com

Website: www.mtc-usa.com