



## Flumazenil USP assay with HPLC – AppNote

### Alternate L1 column used for a similar USP assay method of Flumazenil

This Similar USP Flumazenil is easily performed, and the 10 injections overlay below demonstrates run to run consistency and great peak symmetry. The peak efficiency is very good and peak tailing guidelines are easily met with RSD values of less than 1.0%.

*This demonstrates a good alternate column for your Flumazenil USP method.*

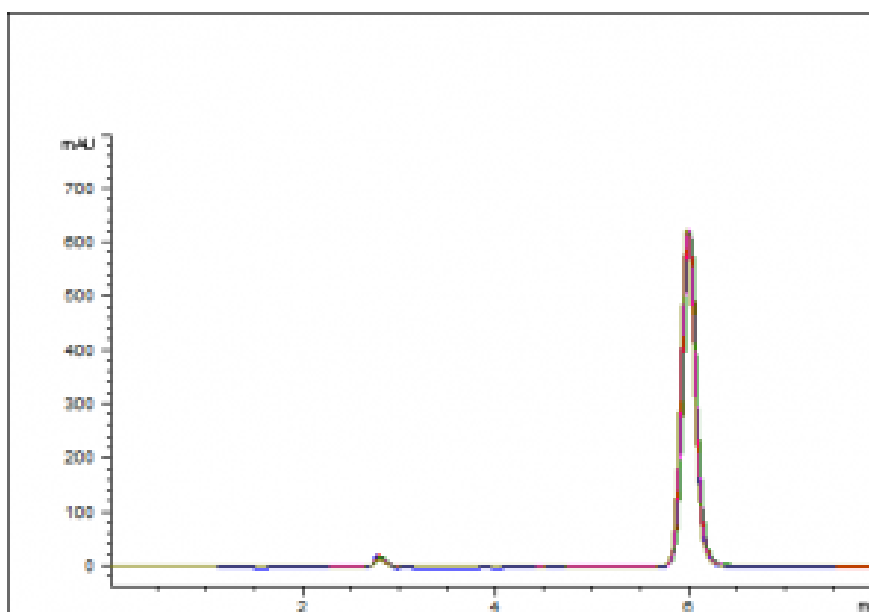

### Peak:

*Flumazenil*

### Method Conditions:

**Column:** Cogent RP C18™, 5µm, 100Å

**Catalog No.:** 68518-15P

**Dimensions:** 4.6mm x 150mm

**Note 1:** For the full method conditions and details, consult the official United States Pharmacopeia–National Formulary (USP–NF.)

**Note 2:** Flumazenil inhibits the action of sodium and potassium ion channels in the heart, which raises the threshold for depolarization and correcting arrhythmias.

Printed from the Chrom Resource Center

Copyright 2024, All Rights Apply

**MicroSolv Technology Corporation**

9158 Industrial Blvd. NE, Leland, NC 28451

tel. (732) 380-8900, fax (910) 769-9435

Email: customers@mtc-usa.com

Website: www.mtc-usa.com

# MICRO**S**OLV

COGENT   
HPLC Columns™

Printed from the Chrom Resource Center

Copyright 2024, All Rights Apply

**MicroSolv Technology Corporation**

9158 Industrial Blvd. NE, Leland, NC 28451

tel. (732) 380-8900, fax (910) 769-9435

Email: [customers@mtc-usa.com](mailto:customers@mtc-usa.com)

Website: [www.mtc-usa.com](http://www.mtc-usa.com)