



Retention of a Tricyclic Amine Analyzed with ELSD-AppNote

Memantine Hydrochloride, a Tricyclic Amine

As this compound lacks Chromophores, it typically requires Derivatization for use in UV detection. In this Method, we retain excellent peak shape without the need for these pre-column derivatization steps.

This compound can also cause issues with Peak Tailing in typical Reversed Phase Columns due to the strong adsorption of residual Silanols. RSD values (less than 0.4%) demonstrate the consistent and reliable Retention.

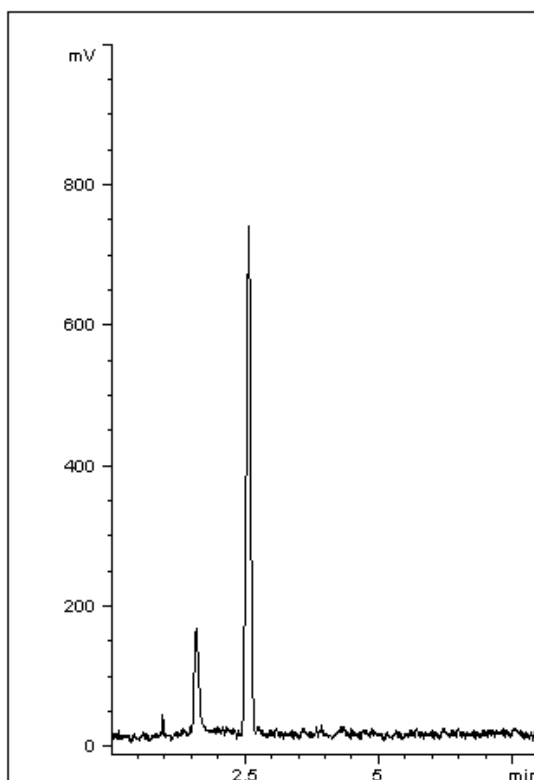

Peak:

Memantine HCl

Method Conditions:

Column: Cogent Diamond Hydride™, 4μm, 100Å.

Catalog No.: 70000-10P

Dimensions: 4.6mm x 100mm

MICROSOLV

Mobile Phase: 95% Acetonitrile / 5% DI Water 10 mM Ammonium Formate

Injection vol.: 1µL

Flow rate: 1.0mL / minute.

Detection: ELSD, Gain: 12, Temperature: 50°C, Nitrogen: 3.5 bar.

Sample Preparation: 1.0mg / mL Mermantine HCL in DI Water.

***Notes:** Persistent activation of the N-methyl-D-aspartate (NMDA) receptors in the central nervous system triggered by glutamate is believed to cause some of the Alzheimer's disease symptoms. Memantine blocks the effects of glutamate, a neurotransmitter in the brain that leads to neuronal excitability and stimulation, being offered as a treatment for Alzheimer's dementia.*



Printed from the Chrom Resource Center

MicroSolv Technology Corporation

9158 Industrial Blvd. NE, Leland, NC 28451

tel. (732) 380-8900, fax (910) 769-9435

Email: customers@mtc-usa.com

Website: www.mtc-usa.com

Date: 05-18-2024