


RSA-Pro X vial improve quantitation precision with HPLC - AppNote

RSA-Pro X™ - Hydrolytically stable hydrophobic glass vials & low volume glass inserts


Silanol groups (Si-OH) on the surface of glass has been known to cause not only empirical quantitative loss but also inaccurate quantitation, vial to vial and run to run over time. Silanol sites are very reactive and can produce among other things, imprecise data, reducing the efforts of the user's preparation and care.

The data below, from our lab, shows the range of quantitative differences in silanized glass vials versus the RSA-Pro X™ vials over 72 hours, in aqueous conditions compared to "silanized" glass.


Vials were prepared with 1ppm of chlorhexidine acetate in a diluent of DI water. Samples analyzed within 24 hours show little no difference of % RSD data, whereas the quantitation over 72 hours illustrate not only that there is some sample loss but that the variability of quantitation in with time worsens and can be more and more problematic.

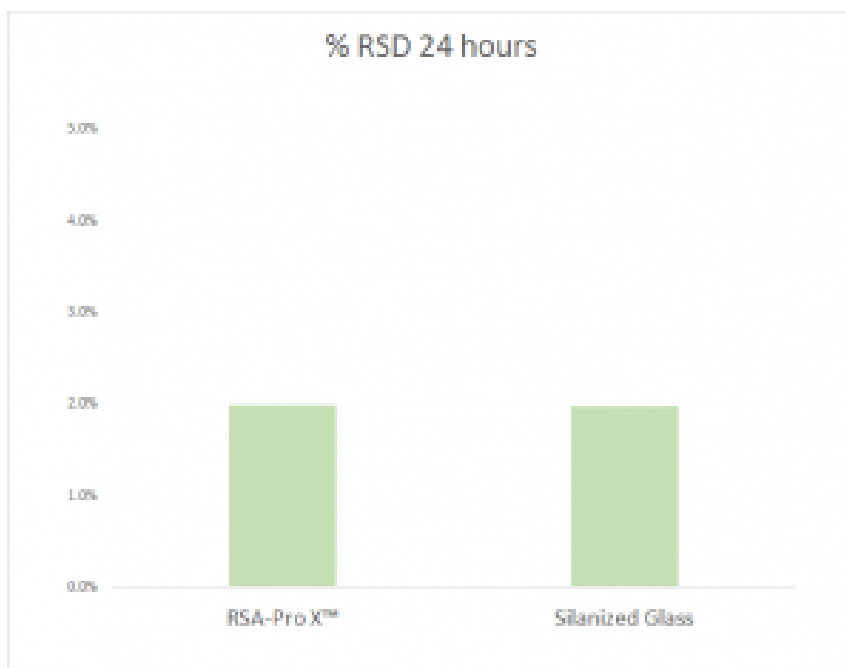

Above chart shows %RSD of Quantitation with RSA-Pro X™ Vials Versus Silanized Glass Vials, post 24 hour exposure. 1 ppm Chlorhexidine Acetate

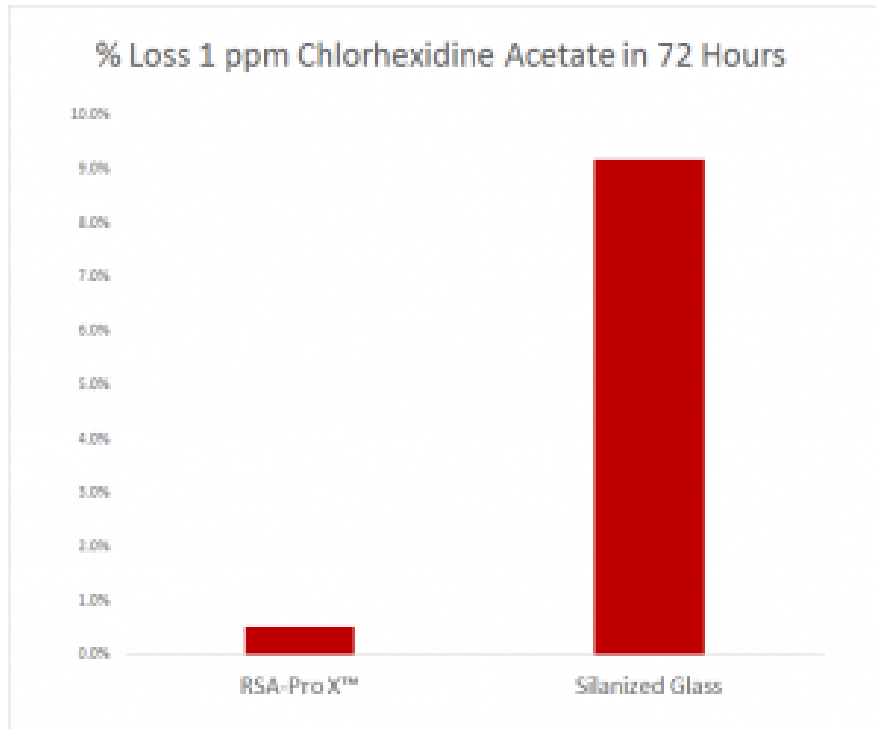

Above chart shows % Loss of Analyte in RSA-Pro X™ Vials Versus Silanized Glass Vials, post 72 hour exposure. 1 ppm Chlorhexidine Acetate

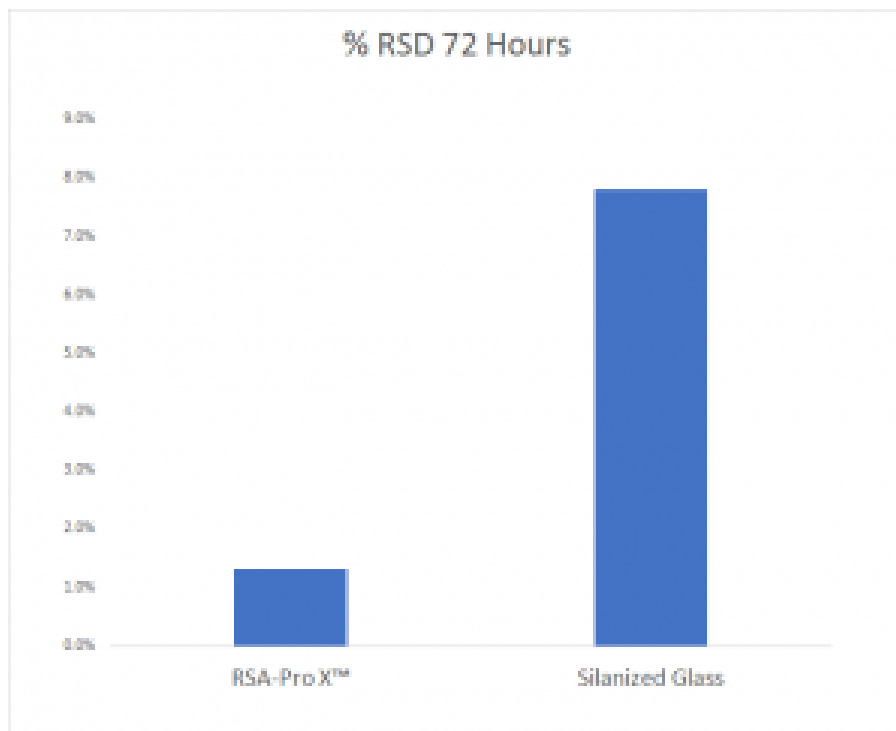

Above chart shows %RSD Quantitation with RSA-Pro X™ Vials Versus Silanized Glass Vials, post 72 hour exposure. 1 ppm Chlorhexidine Acetate

Method Conditions

MICROSOLV

Column: Cogent RP C18™, 5µm, 100Å

Catalog No.: 68518-15P

Dimensions: 4.6 x 150mm

Mobile Phase: 55:45 acetonitrile / buffer (v/v)

Buffer: 0.690g sodium di-hydrogen phosphate, 14.0 g sodium perchlorate, 0.340mL phosphoric acid 50% solution in 1 Liter of DI water.

Injection vol.: 10µL

Flow rate: 1.0mL / minute

Detection: UV @ 260nm

Sample Preparation: 1ppm chlorhexidine acetate in DI water prepared in PPE bottle.

Note: *If you have seen problems with inconsistent coverage from vial to vial or loss of hydrophobicity in water or after 2 weeks, you should consider using the new and advanced technology of RSA-Pro X™ Vial Kits or Inserts. Click [Here](#) for Ordering Information.*

RSA-Pro X™
HYDROLYTIC STABILITY

Printed from the Chrom Resource Center

MicroSolv Technology Corporation

9158 Industrial Blvd. NE, Leland, NC 28451

tel. (732) 380-8900, fax (910) 769-9435

Email: customers@mtc-usa.com

Website: www.mtc-usa.com

Date: 07-22-2024