


## Ticagrelor Analyzed with HPLC – AppNote

### A Reproducible Method for Detection of this Blood Clot Preventative


Click [HERE](#) for Column Ordering Information.

A rapid, sensitive, and Reproducible Method has been developed for analysis of Ticagrelor. The data below, (overlay of 5 chromatograms) illustrates how the compound can be adequately Retained and detected using a simple Gradient in Reversed Phase HPLC. The Method demonstrates good Peak Shape and run-to-run Precision with RSD values less than 0.3%.

A Phenyl ring in the Column Stationary Phase provides beneficial  $\pi$ - $\pi$  Interaction with the Analyte making possible the use of a very simple, Mass Spec friendly Mobile Phase with Formic Acid as an additive.

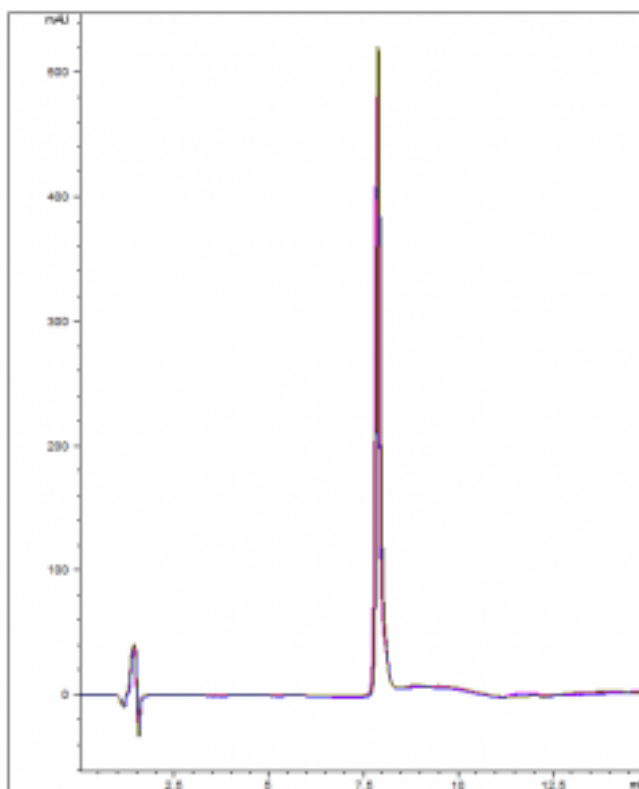

5 Injections of Ticagrelor Overlay

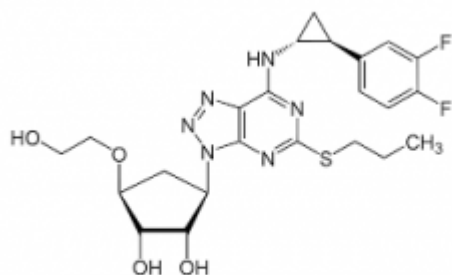

Ticagrelor

Printed from the Chrom Resource Center

Copyright 2024, All Rights Apply

**MicroSolv Technology Corporation**

9158 Industrial Blvd. NE, Leland, NC 28451

tel. (732) 380-8900, fax (910) 769-9435

Email: [customers@mtc-usa.com](mailto:customers@mtc-usa.com)

Website: [www.mtc-usa.com](http://www.mtc-usa.com)

## Method Conditions

**Column:** Cogent Phenyl Hydride™, 4µm, 100Å

**Catalog No.:** 69020-10P-2

**Dimensions:** 2.1mm x 100mm

**Mobile Phase:**

A: DI Water with 0.1% Formic Acid (v/v)

B: Acetonitrile with 0.1% Formic Acid (v/v)

**Gradient:**

Time (minutes)	%B
0	40
1	40
5	85
6	85
7	40
10	40

**Injection vol.:** 1µL

**Flow rate:** 0.2mL / minute

**Detection:** UV @ 254nm

**Sample Preparation:** 2.0mg / mL Ticagrelor standard solution in Methanol.

*Notes: Ticagrelor is an oral prescription indicated for treatment of acute ischemic stroke, coronary artery disease and acute coronary syndrome.*



Printed from the Chrom Resource Center

Copyright 2024, All Rights Apply

**MicroSolv Technology Corporation**

9158 Industrial Blvd. NE, Leland, NC 28451

tel. (732) 380-8900, fax (910) 769-9435

Email: [customers@mtc-usa.com](mailto:customers@mtc-usa.com)

Website: [www.mtc-usa.com](http://www.mtc-usa.com)