
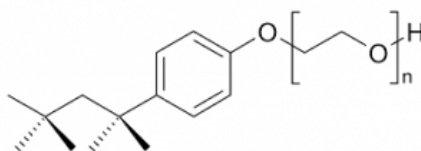


## Triton X-100 gradient assay by HPLC- AppNote

### A reproducible assay for detection of a non-ionic surfactant.

Triton X-100 is used in the sample purification steps of various materials as well as for cleaning apparatus in pharmaceutical manufacturing. Detection and quantification are very important to identify any residual amounts of this compound.

The overlay of 5 injections (below) demonstrates reproducibility in separating the polyoxyethylene mixture.

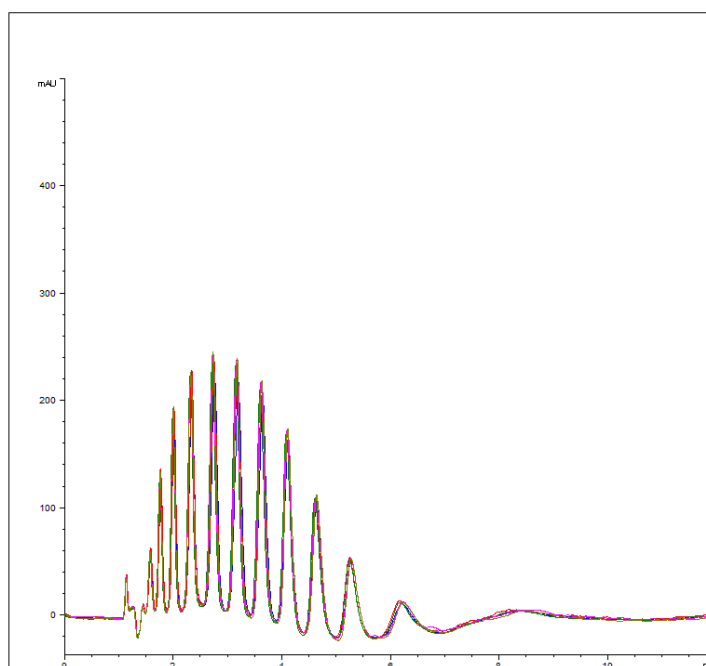

### Peak:

Triton X-100

### Method Conditions:

**Column:** Cogent Bidentate C8™, 4µm, 100Å

**Catalog No.:** 40008-10P

**Dimensions:** 4.6 x 100mm

### Mobile Phase:

A: DI water with 0.1% formic acid

B: Acetonitrile with 0.1% formic acid

Time (minutes)	%B
0	98
2	95
3	95

# MICROSOLV

5	95
10	98

**Injection vol.:** 1µL

**Flow rate:** 1.0mL / minute

**Detection:** UV @ 230nm

**Sample Preparation:** Triton X-100, 10uL / mL in DI water

**Note:** Triton X-100 is one of the most widely used nonionic surfactants for lysing cells to extract protein and other cellular organelles. Triton X-100 ( $C_{14}H_{22}O(C_2H_4O)_n$ ) has a hydrophilic polyethylene oxide chain and an aromatic hydrocarbon lipophilic or hydrophobic group. The hydrocarbon group is a 4-phenyl group.



Printed from the Chrom Resource Center

**MicroSolv Technology Corporation**

9158 Industrial Blvd. NE, Leland, NC 28451

tel. (732) 380-8900, fax (910) 769-9435

Email: [customers@mtc-usa.com](mailto:customers@mtc-usa.com)

Website: [www.mtc-usa.com](http://www.mtc-usa.com)

Date: 07-22-2024