



Domoic Acid analyzed by LCMS - AppNote

Determination without derivatization

To date, several analytical methods have been developed for the quantitative determination of Domoic Acid (DA). However, many of the methods require tedious and labor intensive derivatization of this compound in order to detect it.

A new method based on HPLC and MS detection which does not require derivatization has been developed. A simple linear gradient and typical MS compatible mobile phases were used to retain DA, a potent Neurotoxin.

The method can be used by regulatory agencies responsible for monitoring the occurrence of toxins for analysis of Domoic Acid in seafood samples and other laboratories.

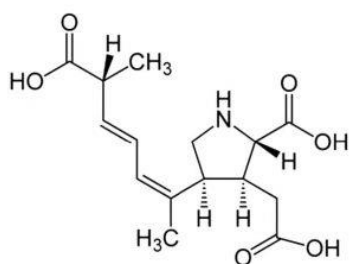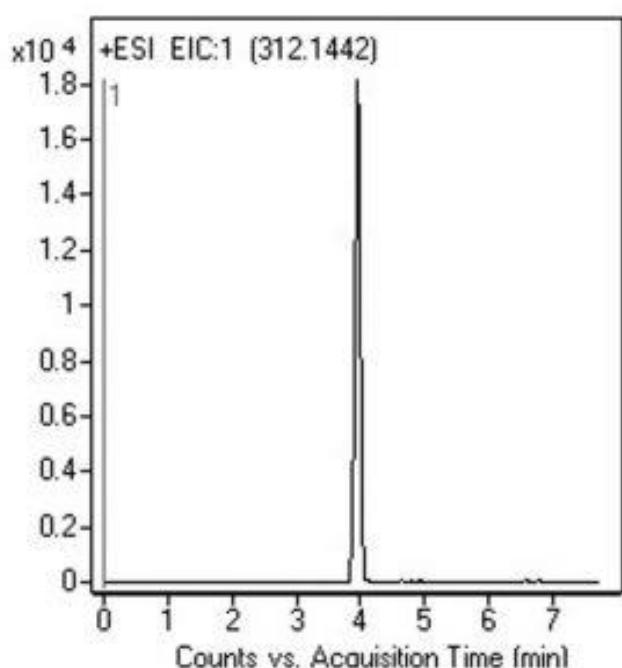

Peak:

Domoic Acid 312.1442 m/z (M + H)⁺

Method Conditions

Column: Cogent Diamond Hydride™, 4µm, 100Å

Catalog No.: [70000-05P-2](#)

Dimensions: 2.1 x 50mm

Mobile Phase:

A: 50% Methanol / 50% DI Water / 0.1% Formic Acid

B: 97% Acetonitrile / 3% DI Water / 0.1% Formic Acid

Gradient:

Time (minutes)	%B
0	95
10	30
11	30
12	95

Post Time: 5 minutes

Flow rate: 0.4 mL / minute

Detection: ESI – POS – Agilent 6210 MSD TOF Mass Spectrometer

Injection vol.: 1µL

Sample Preparation:

Stock Solution: 1mg / mL in Methanol diluent.

Working Solution: Stock aliquot was diluted using 50% Solvent A and 50% Solvent B mixture for the final concentration 0.5mg / L. Before injection, solution was filtered using a 0.45µm Nylon Syringe Filter (MicroSolv Tech Corp.).

Note: Domoic Acid, a compound known for over 50 years, was found to have neurological effects when ingested by humans. It is the chemical responsible for amnesiac shellfish poisoning (ASP). Upon ingestion by humans, it can cause diarrhea, dizziness, seizures, permanent loss of short-term memory, and even death. In Canada, the European Union, and the USA, the legal limit is 20 µg DA / g in wet tissues of shellfish.



Attachment

Domoic Acid by LCMS pdf [Download File](#)

Printed from the Chrom Resource Center
Copyright 2025, All Rights Apply
MicroSolv Technology Corporation
9158 Industrial Blvd. NE, Leland, NC 28451

Tel: (732) 380-8900
Fax: (910) 769-9435
Email: customers@mtc-usa.com
Website: www.mtc-usa.com